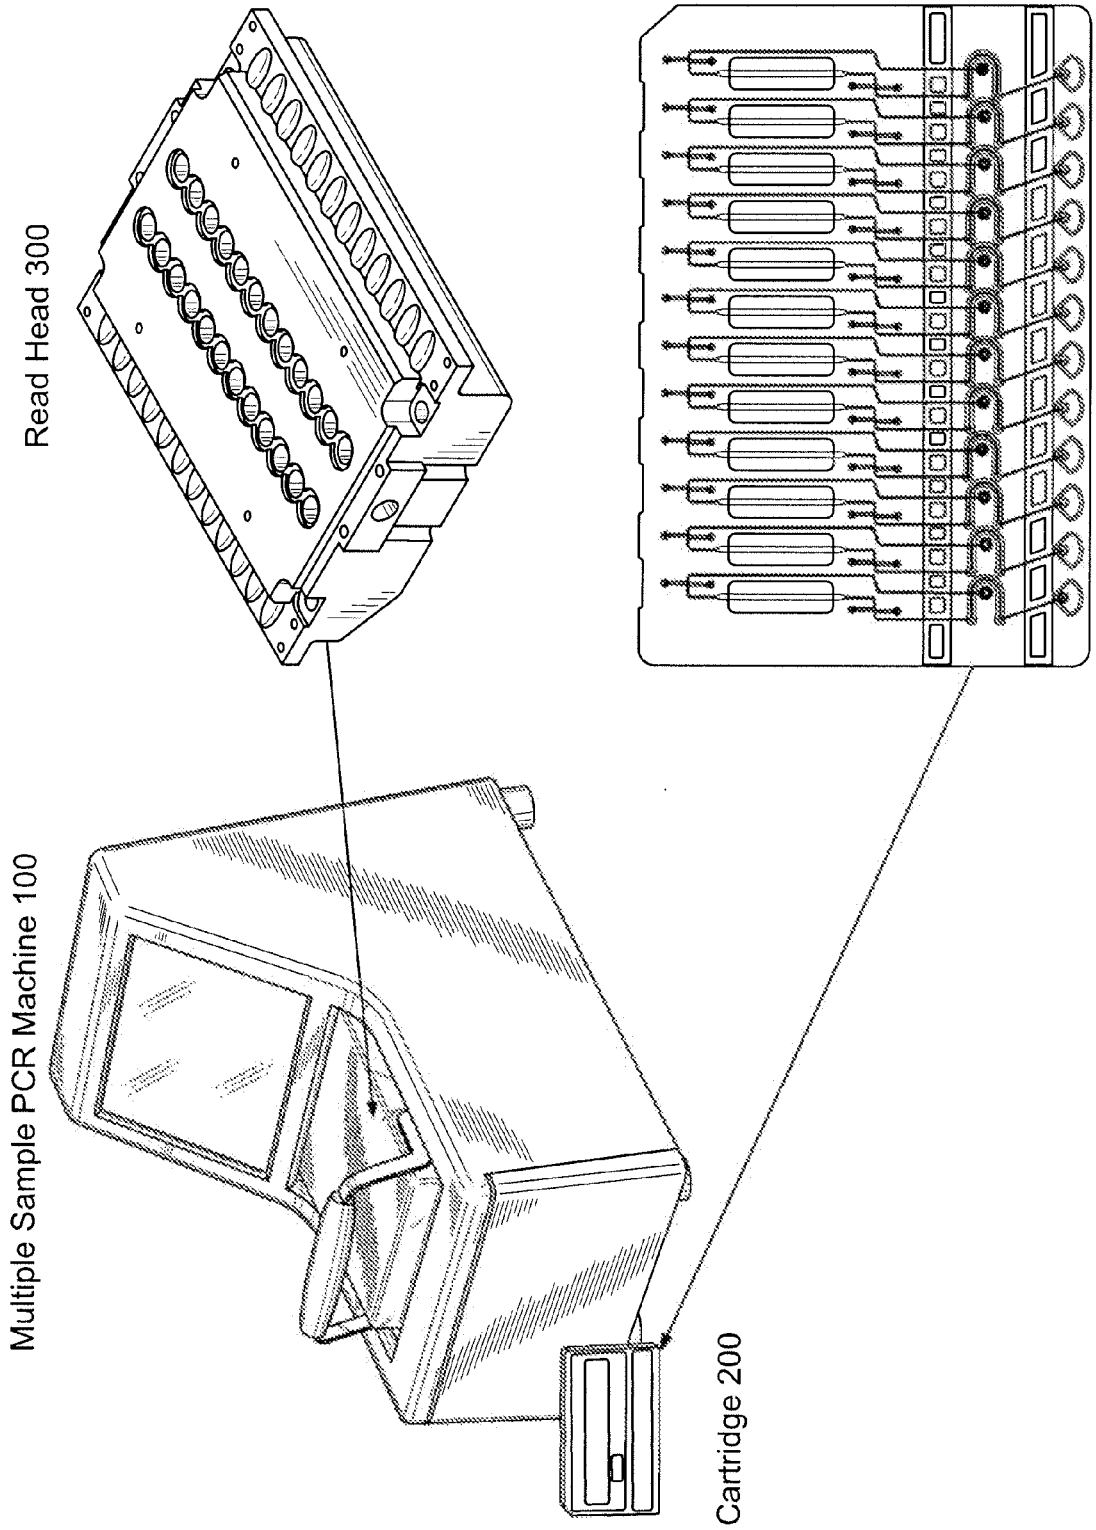
Read Head 300
Multiple Sample PCR Machine 100
Cartridge 200

FIG. 1