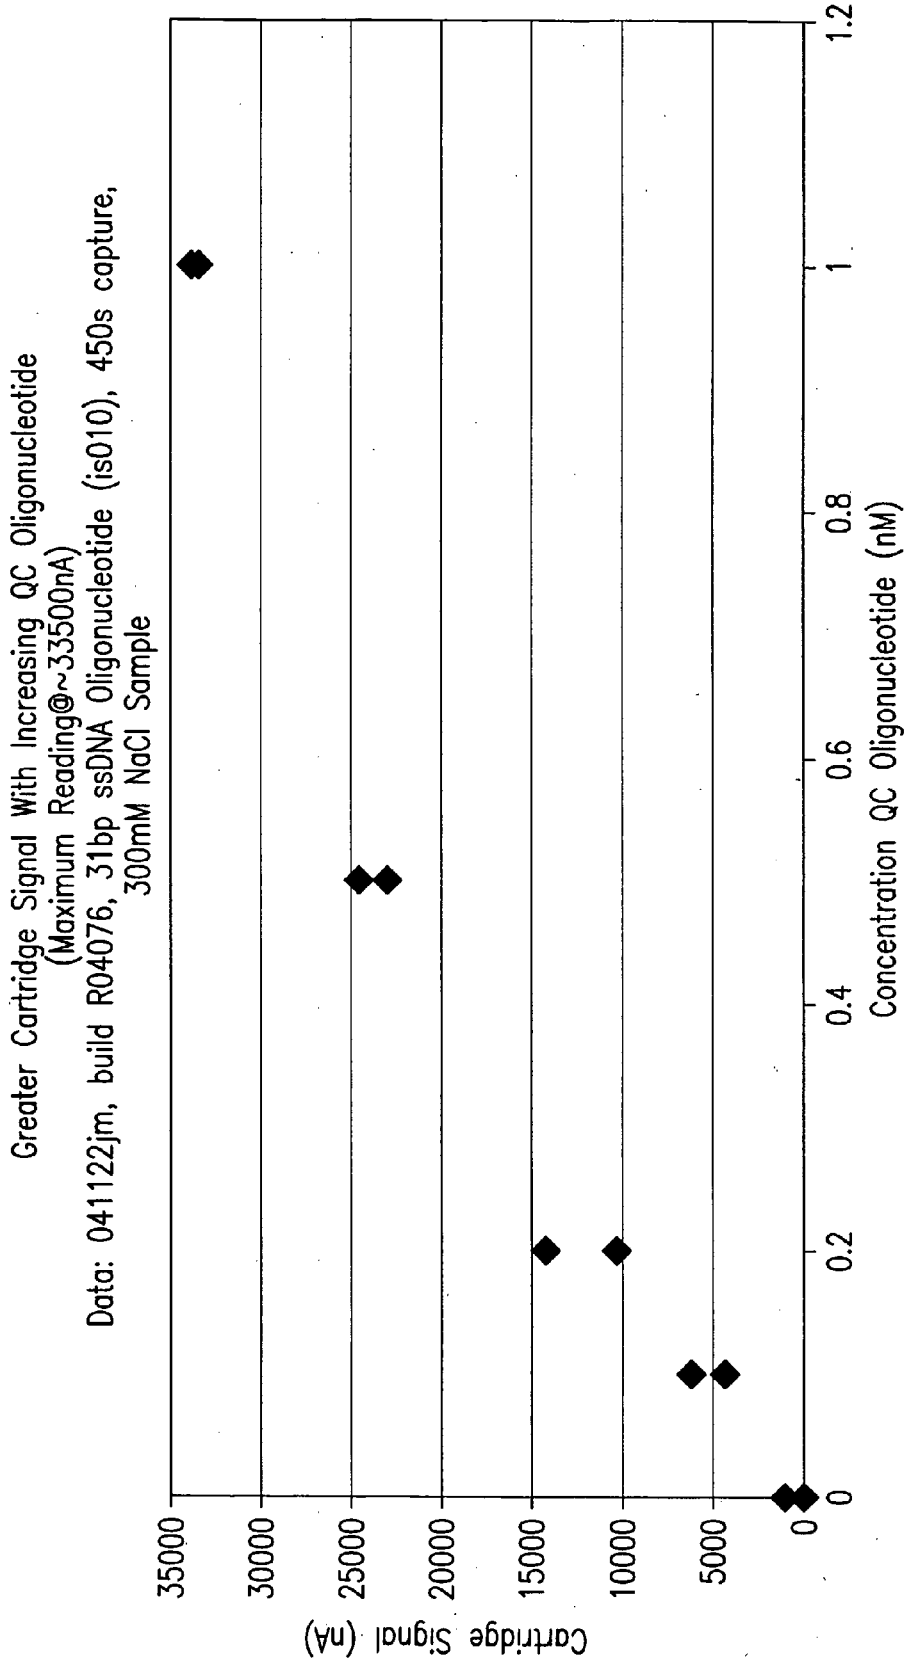
Greater Cartridge Signal With Increasing QC Oligonucleotide
(Maximum Reading@~33500nA)
Data: 041122jm, build R04076, 31bp ssDNA Oligonucleotide (is010), 450s capture,
300mM NaCl Sample
Cartridge Signal (nA)
35000
30000
25000
20000
15000
10000
5000
0
0
0.2
0.4
0.6
0.8
1
1.2
Concentration QC Oligonucleotide (nM)

FIG.29B