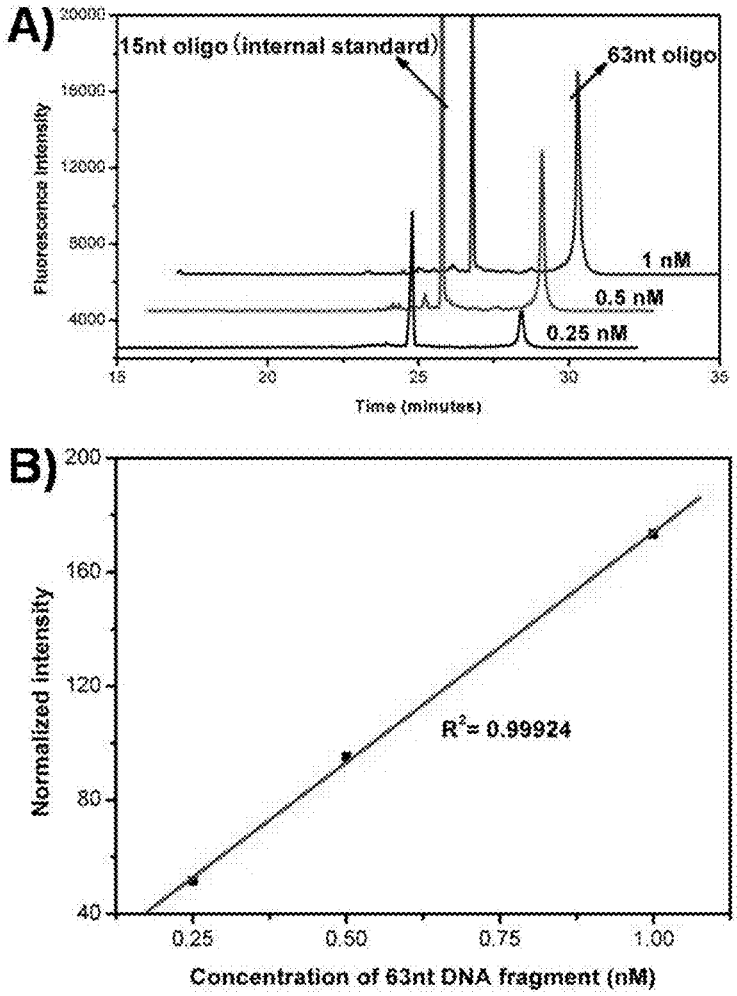
A)
15nt oligo (internal standard)
63nt oligo
1 nM
0.5 nM
0.25 nM
Fluorescence Intensity
Time (minutes)
B)
Normalized intensity
R^2= 0.99924
Concentration of 63nt DNA fragment (nM)

FIGURE 7A-B