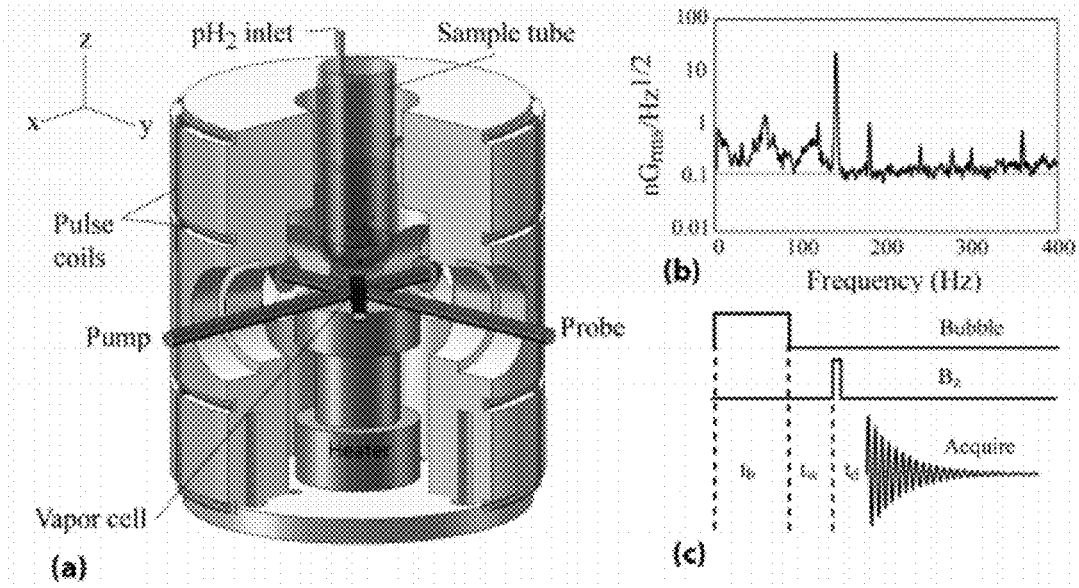
z
x
y
pH2 inlet
Sample tube
Pulse coils
Pump
Probe
Vapor cell
(a)
100
10
1
0.1
0.01
nG_rms/Hz^1/2
0
100
200
300
400
Frequency (Hz)
(b)
Bubble
B0
Acquire
(c)

Figure 7