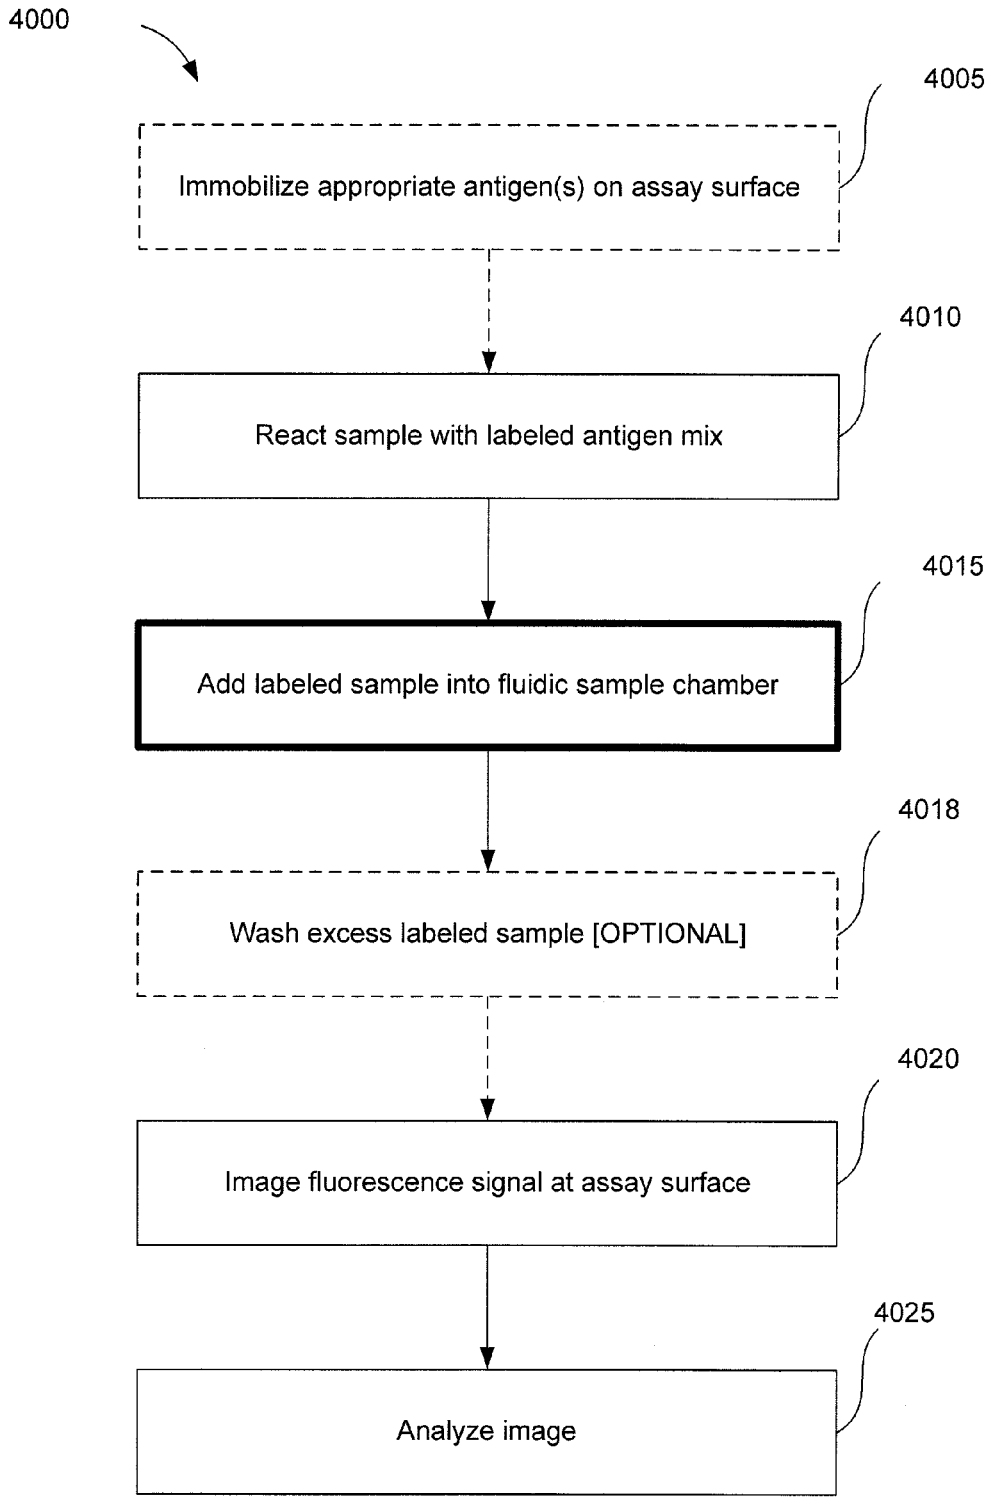
4000
4005
Immobilize appropriate antigen(s) on assay surface
4010
React sample with labeled antigen mix
4015
Add labeled sample into fluidic sample chamber
4018
Wash excess labeled sample [OPTIONAL]
4020
Image fluorescence signal at assay surface
4025
Analyze image

FIG. 40