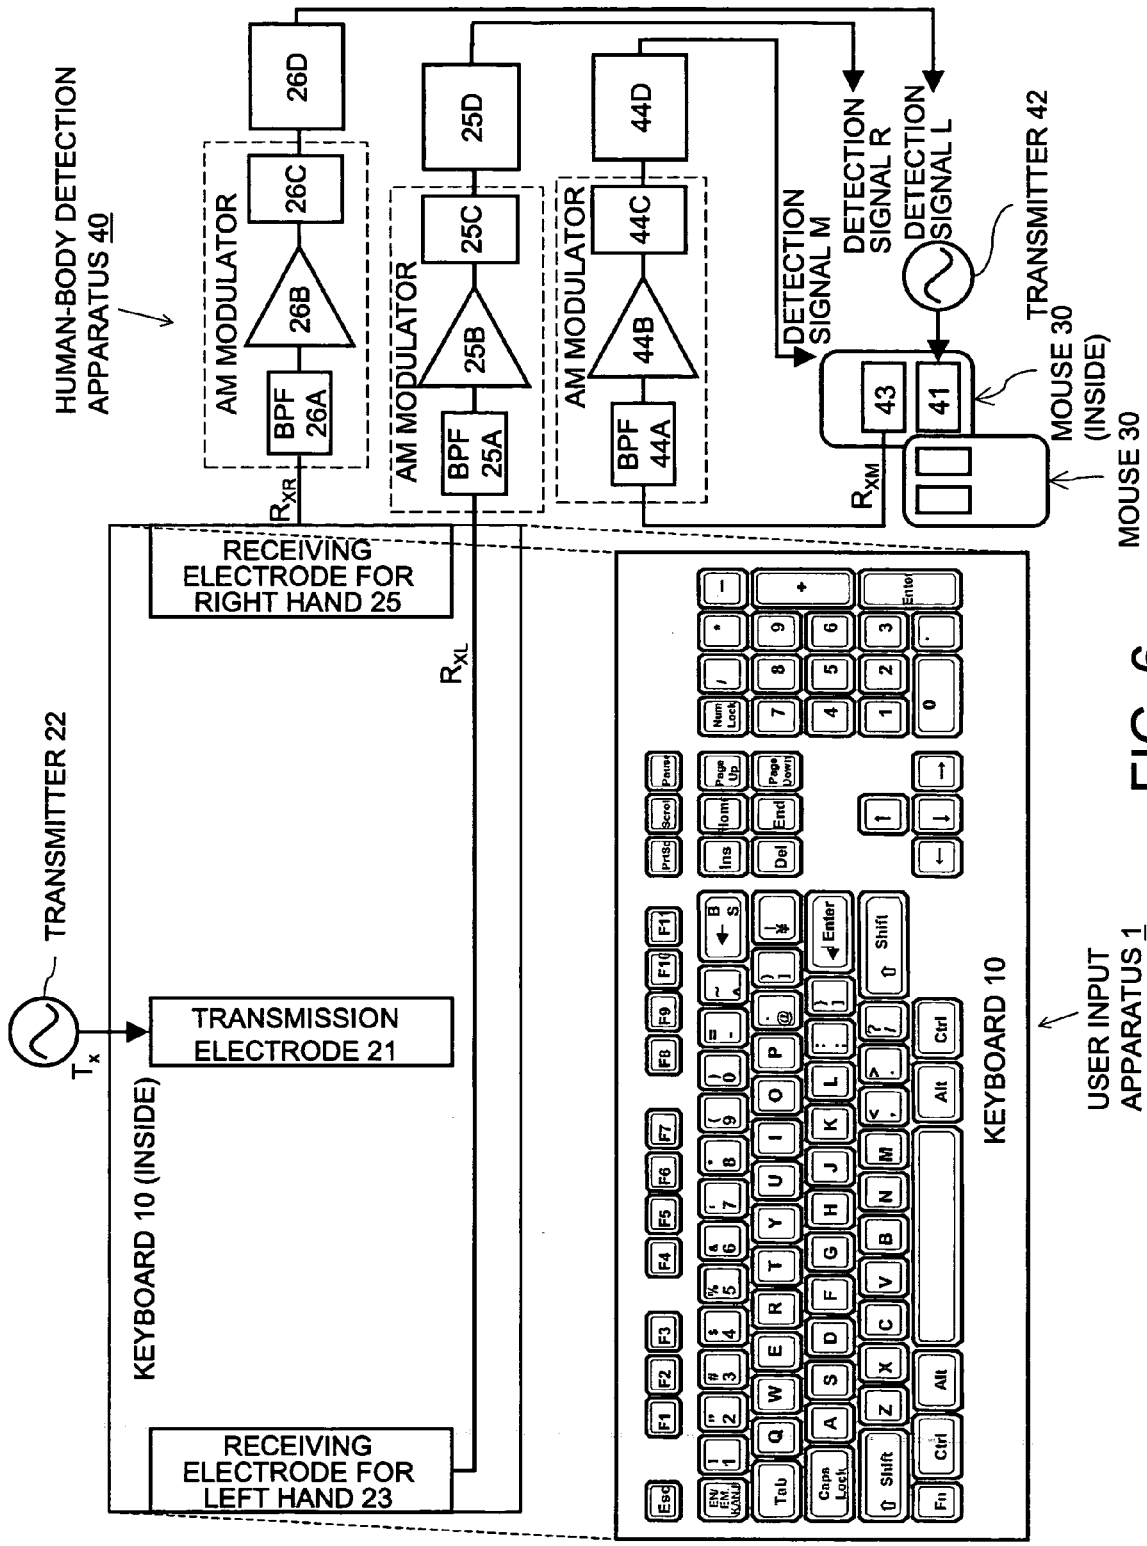
HUMAN-BODY DETECTION APPARATUS 40
AM MODULATOR
BPF 26A
26B
26C
26D
AM MODULATOR
BPF 25A
25B
25C
25D
AM MODULATOR
BPF 44A
44B
44C
44D
DETECTION SIGNAL M
DETECTION SIGNAL R
DETECTION SIGNAL L
TRANSMITTER 42
43
41
MOUSE 30 (INSIDE)
MOUSE 30
R_{XR}
R_{XL}
R_{XM}
RECEIVING ELECTRODE FOR RIGHT HAND 25
RECEIVING ELECTRODE FOR LEFT HAND 23
TRANSMITTER 22
T_x
TRANSMISSION ELECTRODE 21
KEYBOARD 10 (INSIDE)
KEYBOARD 10
USER INPUT APPARATUS 1

FIG. 6