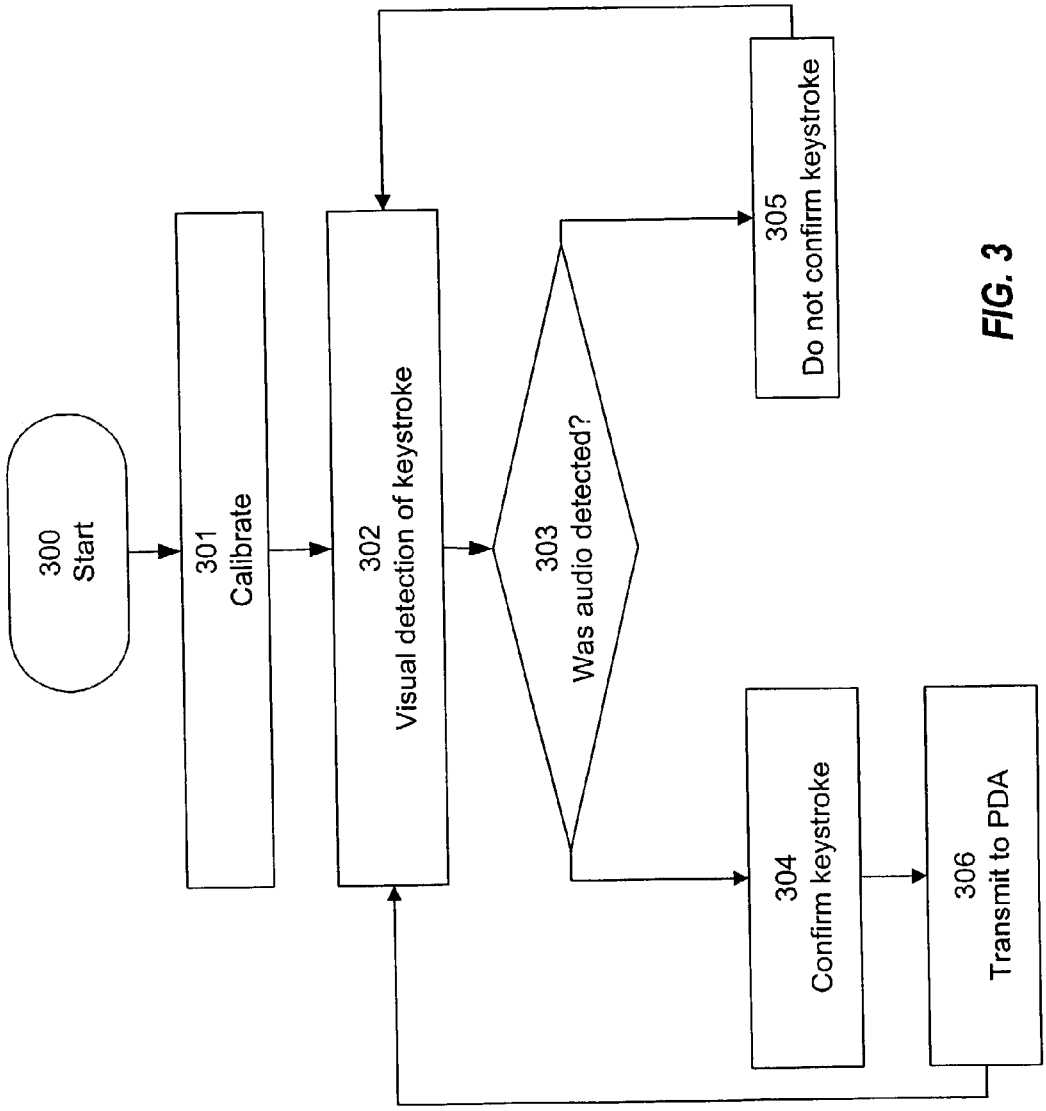
300
Start
301
Calibrate
302
Visual detection of keystroke
303
Was audio detected?
304
Confirm keystroke
305
Do not confirm keystroke
306
Transmit to PDA

FIG. 3