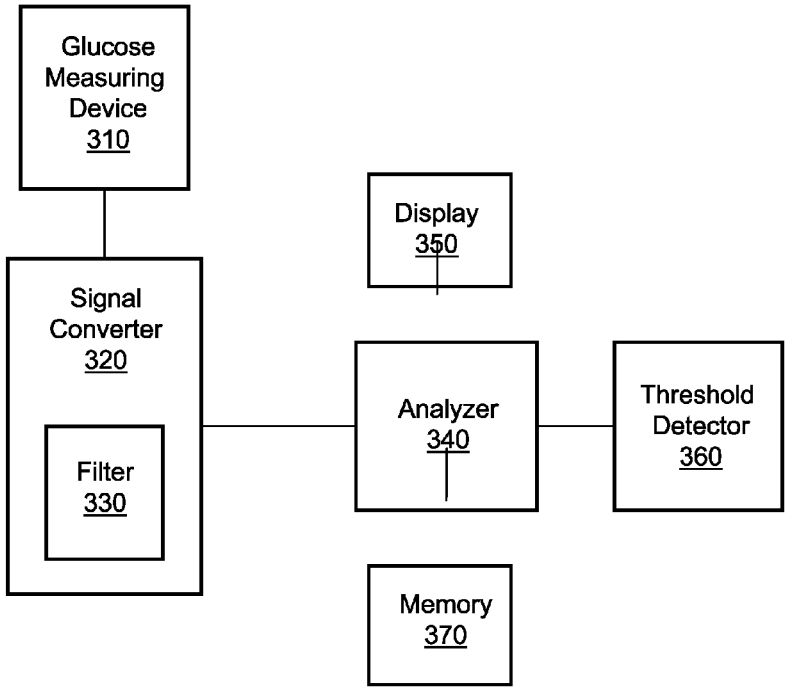

FIG. 2B

CGM Device	Manufacturing Company	# of Subjects	Diabetes Type	Sampling Interval (min)	Collection Time (days)
iSense	iSense Corp	9	1	1	5
Guardian RT	Medtronic Inc	18	1	5	6
DexCom	DexCom Inc	7	2	5	56

FIG. 3