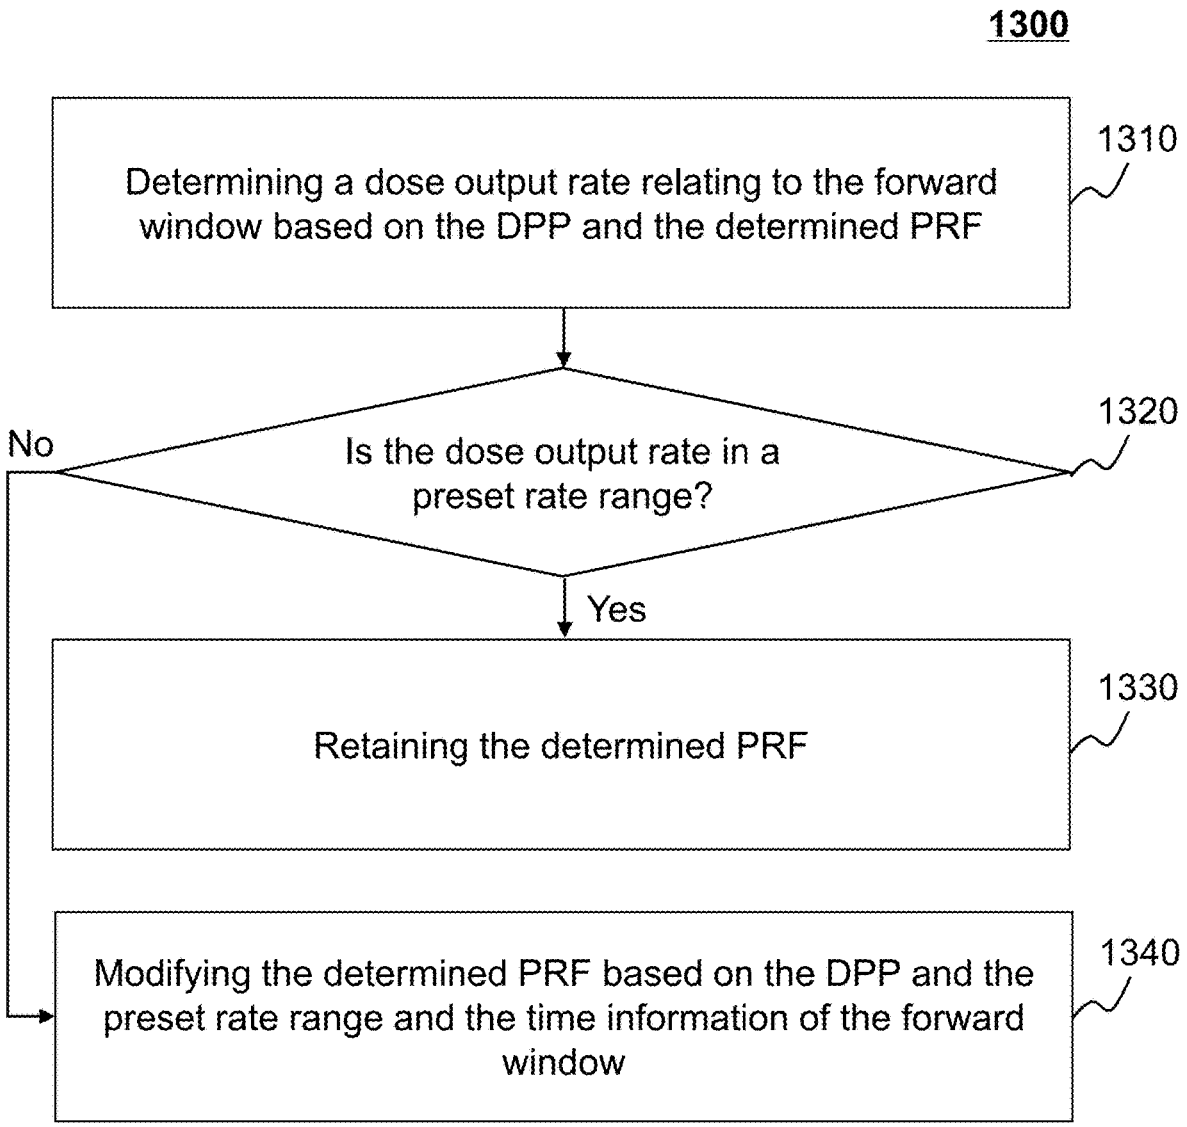
1300
Determining a dose output rate relating to the forward window based on the DPP and the determined PRF
1310
Is the dose output rate in a preset rate range?
1320
No
Yes
Retaining the determined PRF
1330
Modifying the determined PRF based on the DPP and the preset rate range and the time information of the forward window
1340

FIG. 13