




US 20190122768A1

(19) **United States**(12) **Patent Application Publication**  
**PULITZER et al.**(10) **Pub. No.: US 2019/0122768 A1**(43) **Pub. Date: Apr. 25, 2019**(54) **SYSTEM AND METHOD FOR A DIGITAL  
CONSUMER MEDICAL WALLET AND  
STOREHOUSE**(71) Applicant: **RELIANT IMMUNE  
DIAGNOSTICS, INC.**, Austin, TX  
(US)(72) Inventors: **JOVAN HUTTON PULITZER**,  
FRISCO, TX (US); **HENRY JOSEPH  
LEGERE, III**, AUSTIN, TX (US)(21) Appl. No.: **16/137,204**(22) Filed: **Sep. 20, 2018****Related U.S. Application Data**(63) Continuation-in-part of application No. 15/804,990,  
filed on Nov. 6, 2017, which is a continuation-in-part  
of application No. 15/295,398, filed on Oct. 17, 2016,  
now Pat. No. 9,857,373.(60) Provisional application No. 62/566,598, filed on Oct.  
2, 2017, provisional application No. 62/419,382, filed  
on Nov. 8, 2016.**Publication Classification**(51) **Int. Cl.****G16H 50/30** (2006.01)**G06Q 30/02** (2006.01)**G16H 10/65** (2006.01)**G06T 7/00** (2006.01)**H04N 5/232** (2006.01)**G01N 33/53** (2006.01)(52) **U.S. Cl.**CPC ..... **G16H 50/30** (2018.01); **G06Q 30/0267**(2013.01); **G06Q 30/0269** (2013.01); **G06F****3/0482** (2013.01); **G06T 7/0014** (2013.01);**H04N 5/23222** (2013.01); **G01N 33/5302**(2013.01); **G16H 10/65** (2018.01)

(57)

**ABSTRACT**

A system and method are provided for collection and testing of a biologic sample. The system and method comprise collecting by a user of a testing device a biologic sample for use with the testing device, assigning correlative values as test results, and receiving the test results at a server disposed on a network. Some aspects further include presenting advertisements and other messages to users through a mobile application operating on a mobile device. These aspects take into account the results of the self-diagnostic test and present different advertisements to the user based on the results of the test.

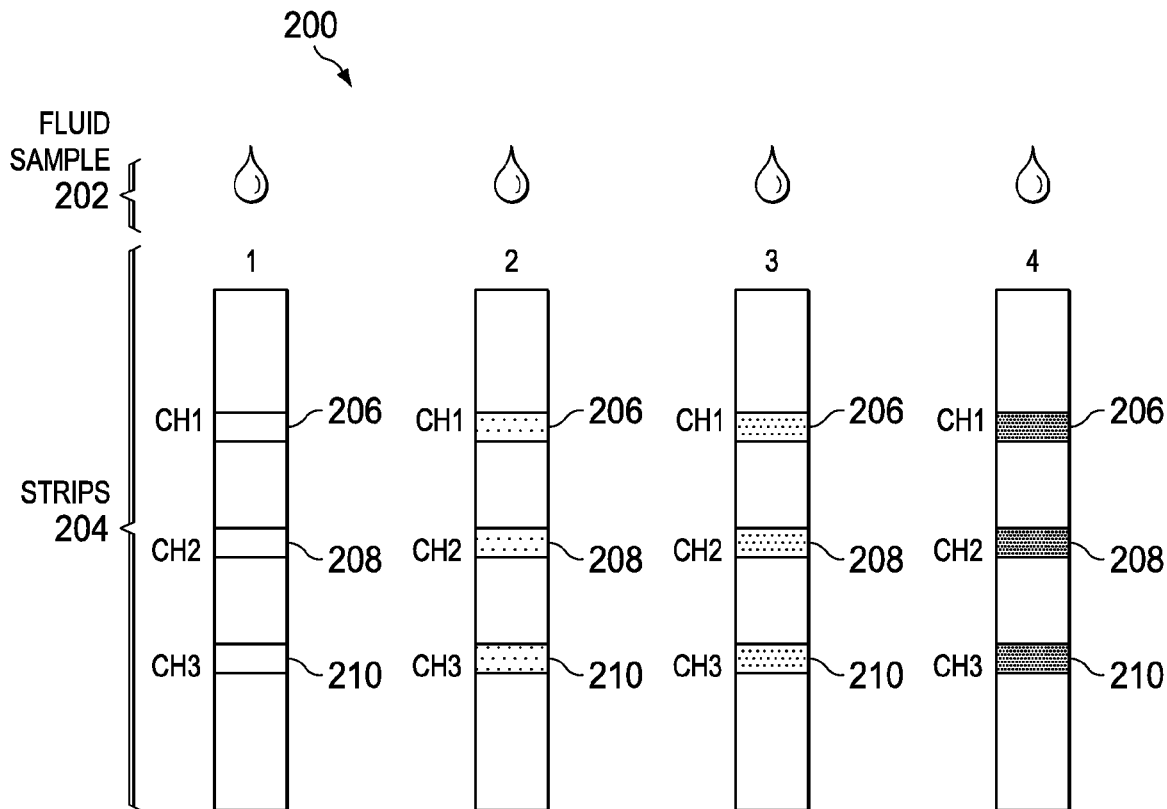

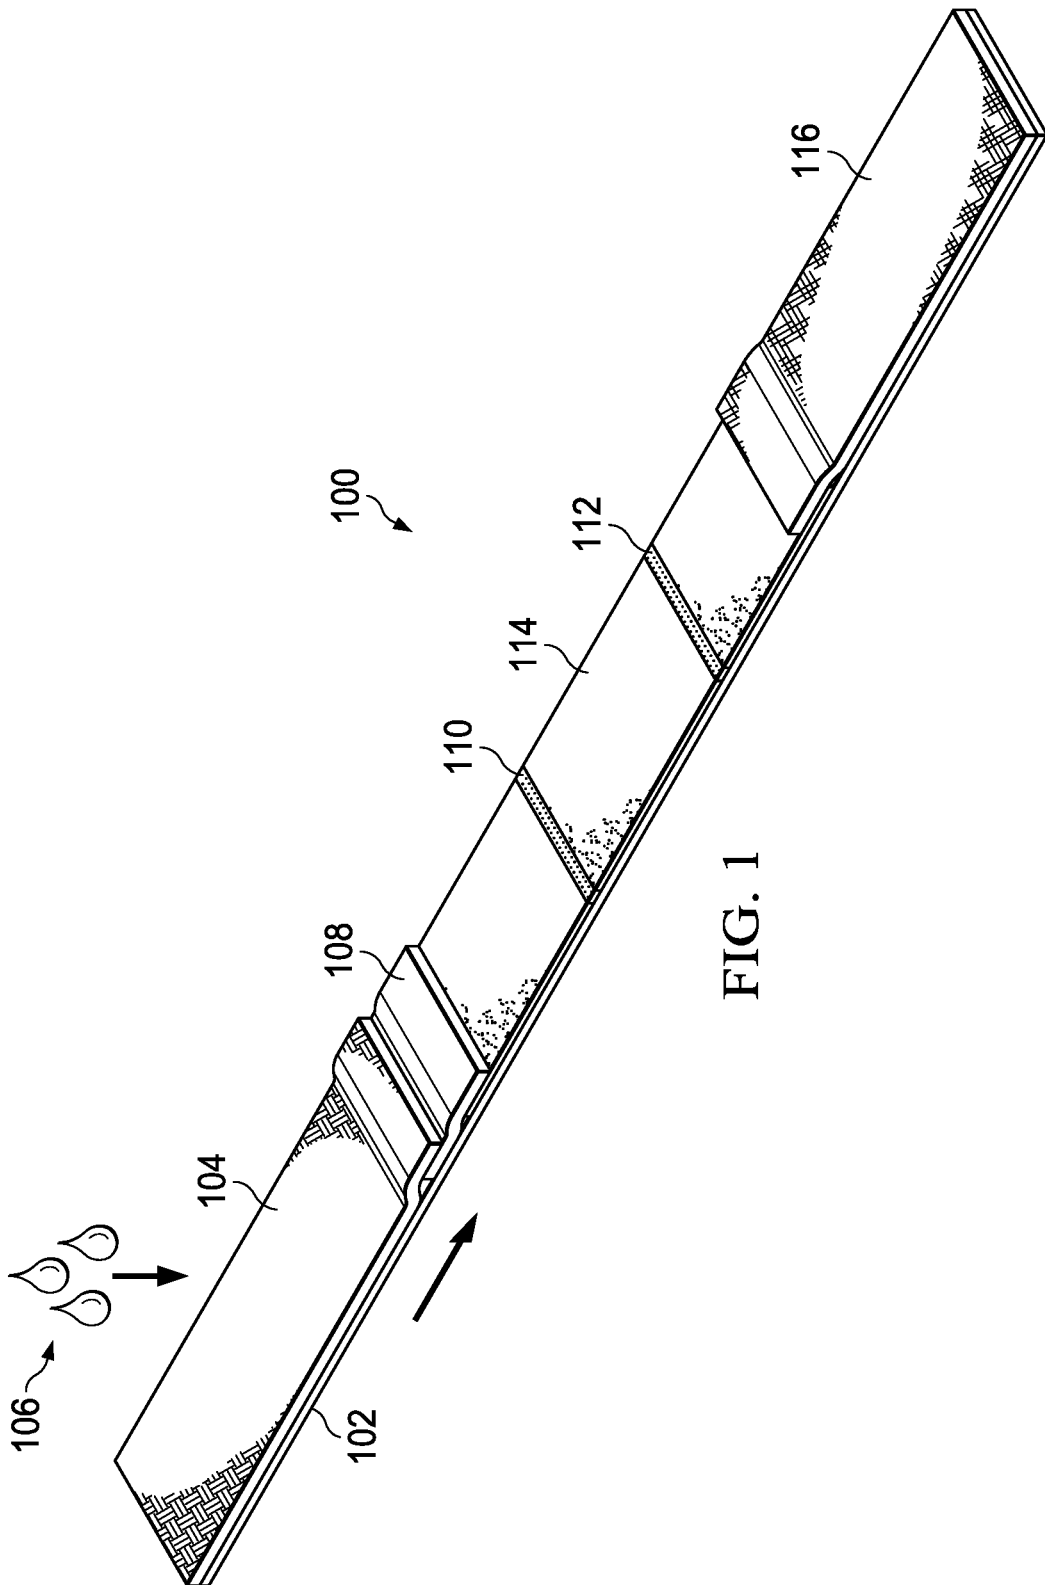


FIG. 1

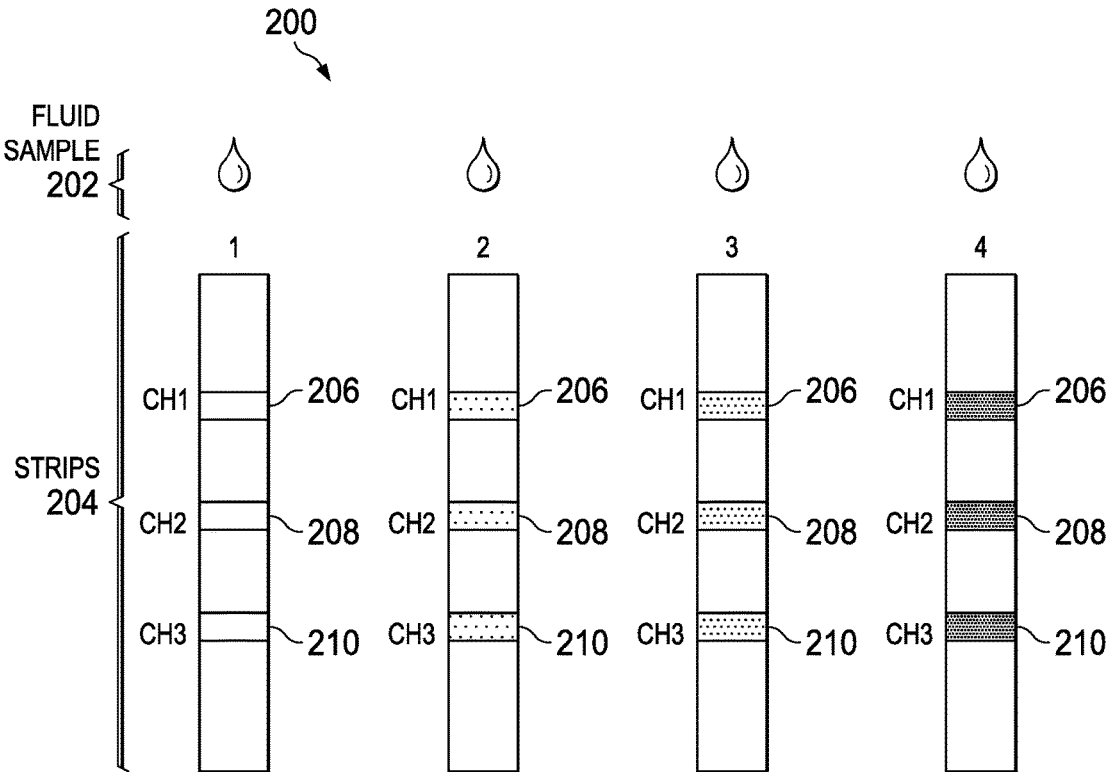


FIG. 2

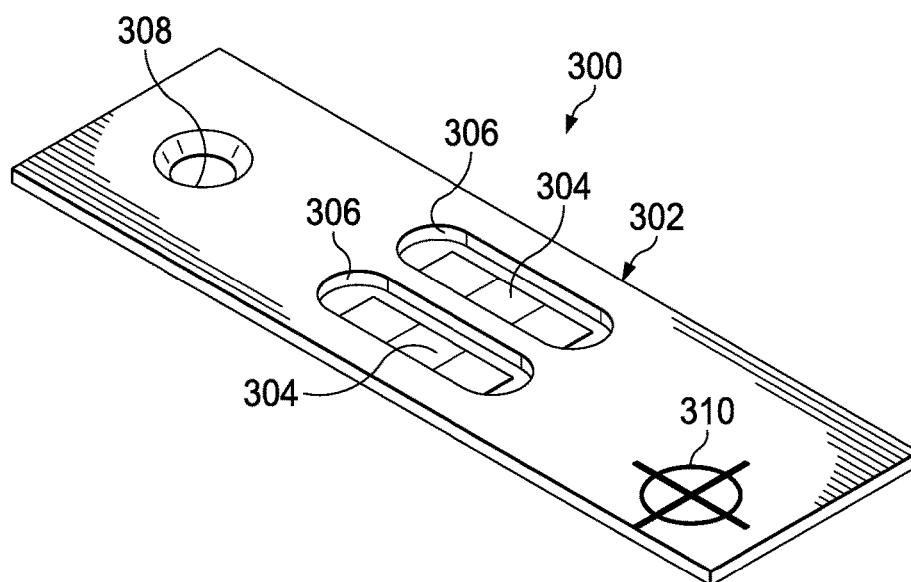


FIG. 3

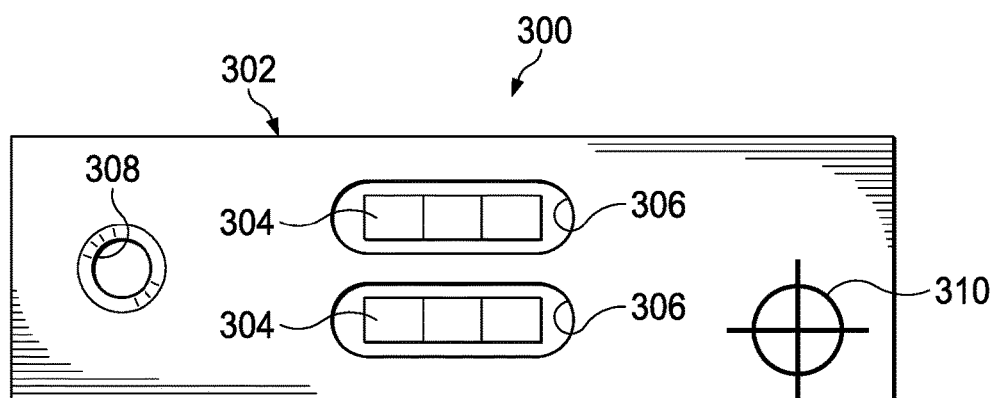


FIG. 4

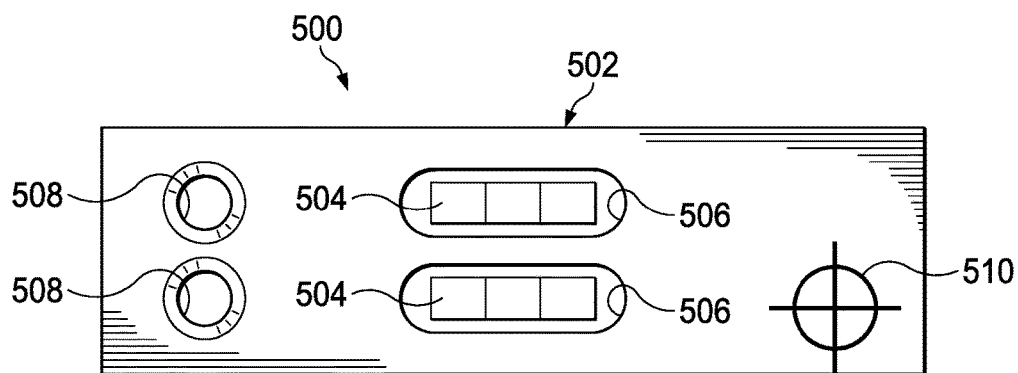


FIG. 5

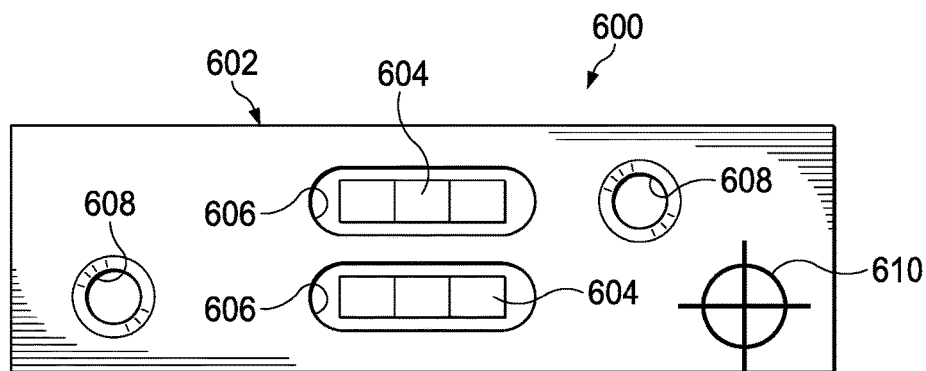


FIG. 6

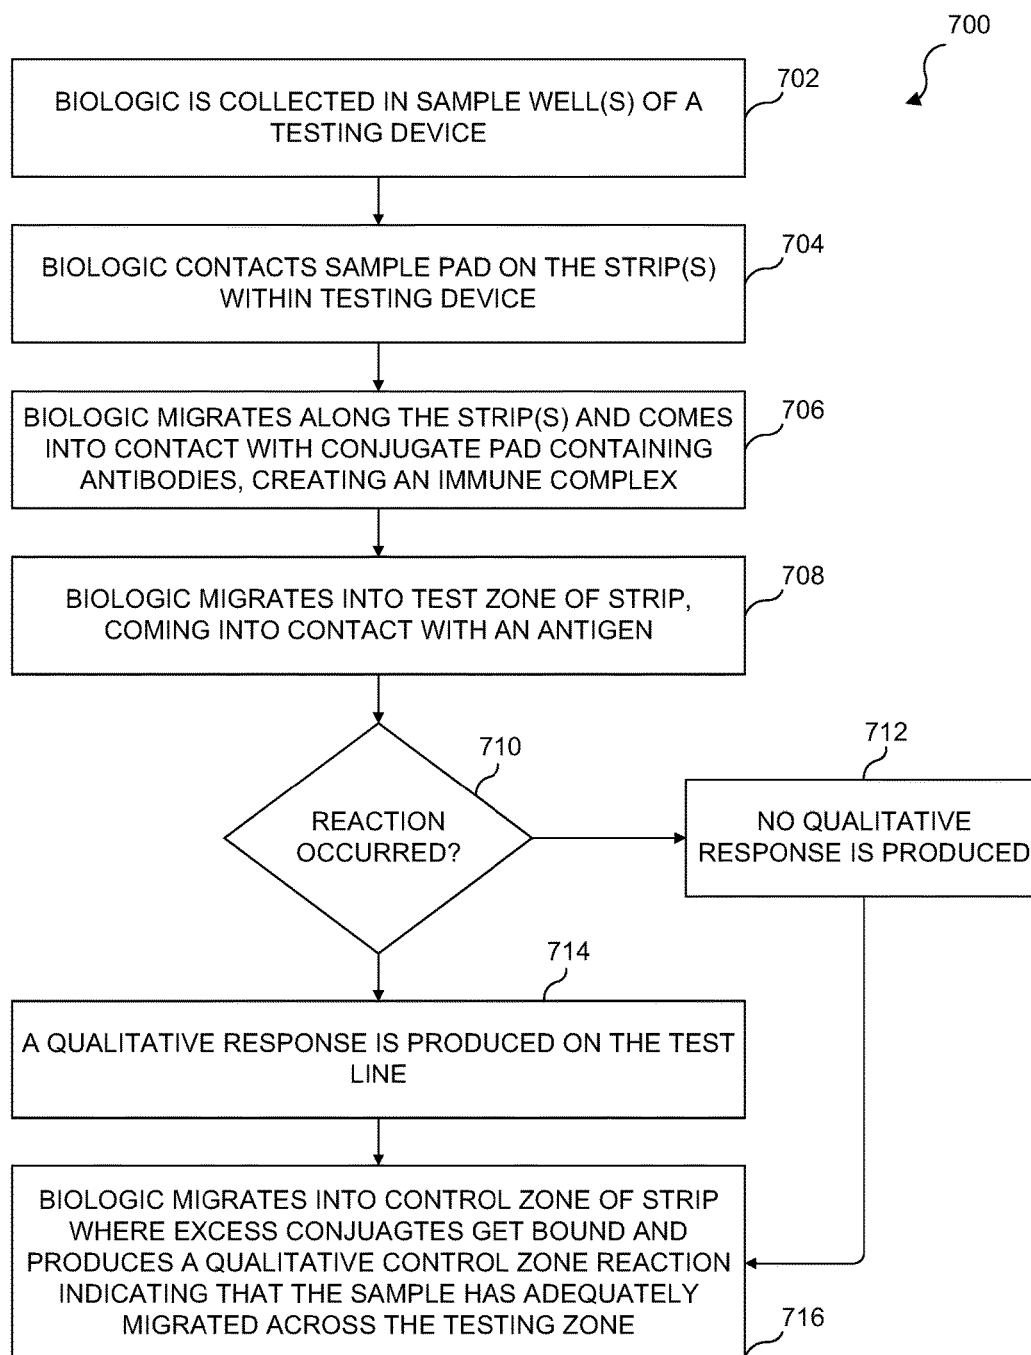


FIG. 7

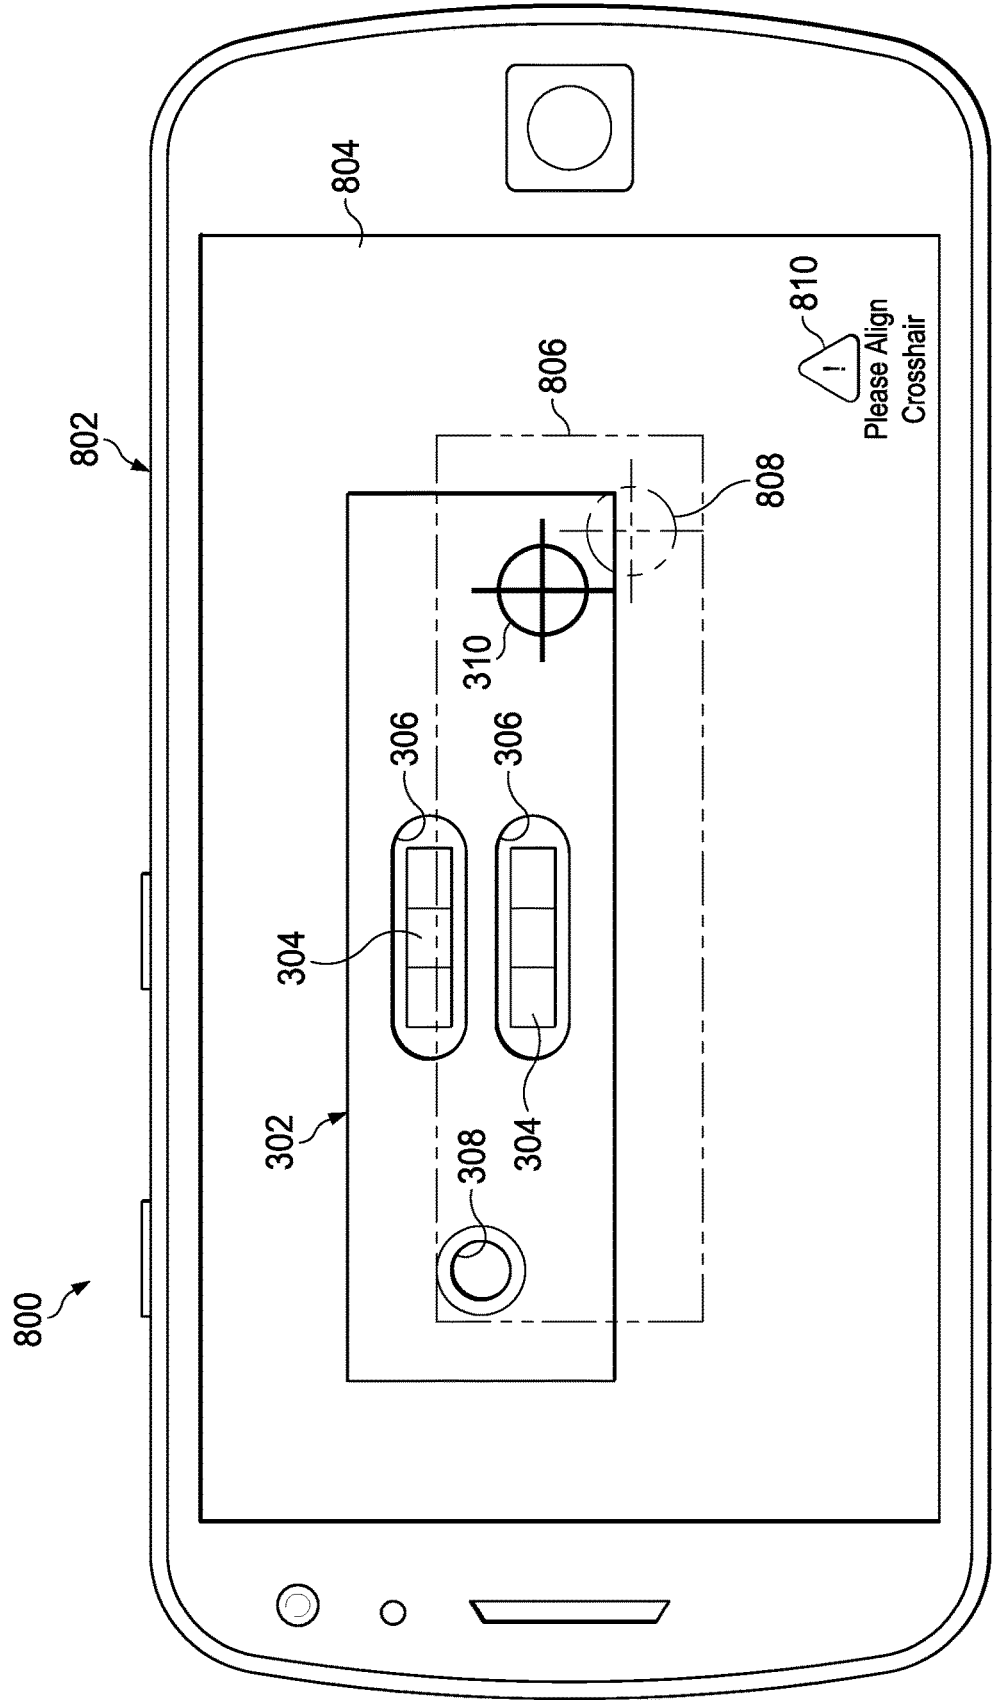


FIG. 8A

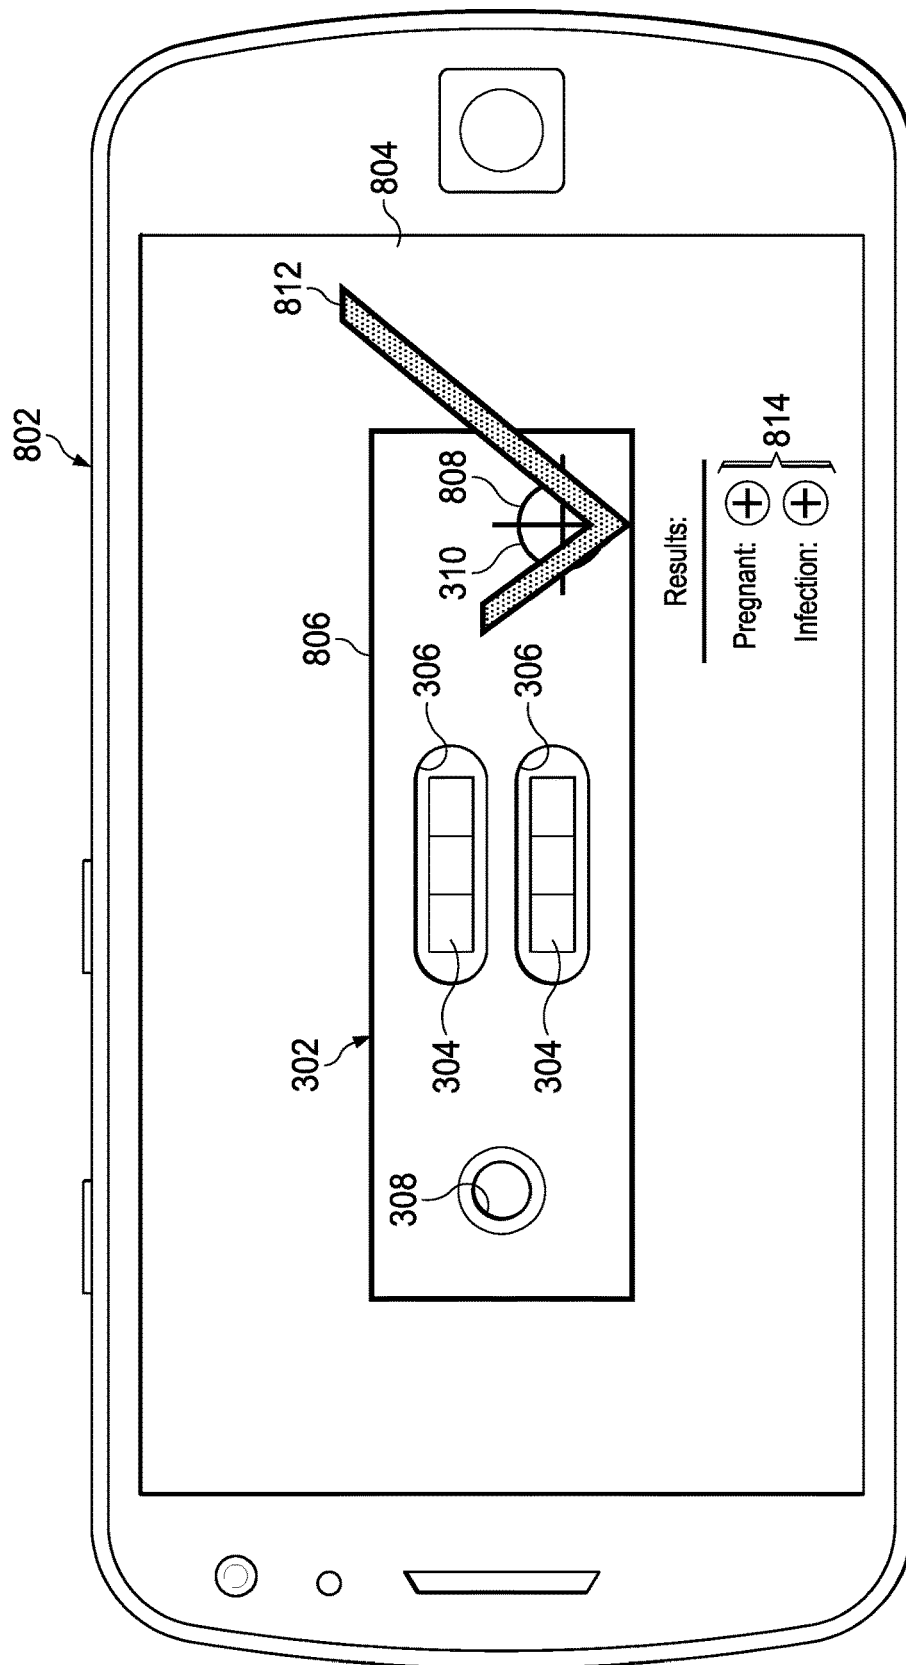


FIG. 8B



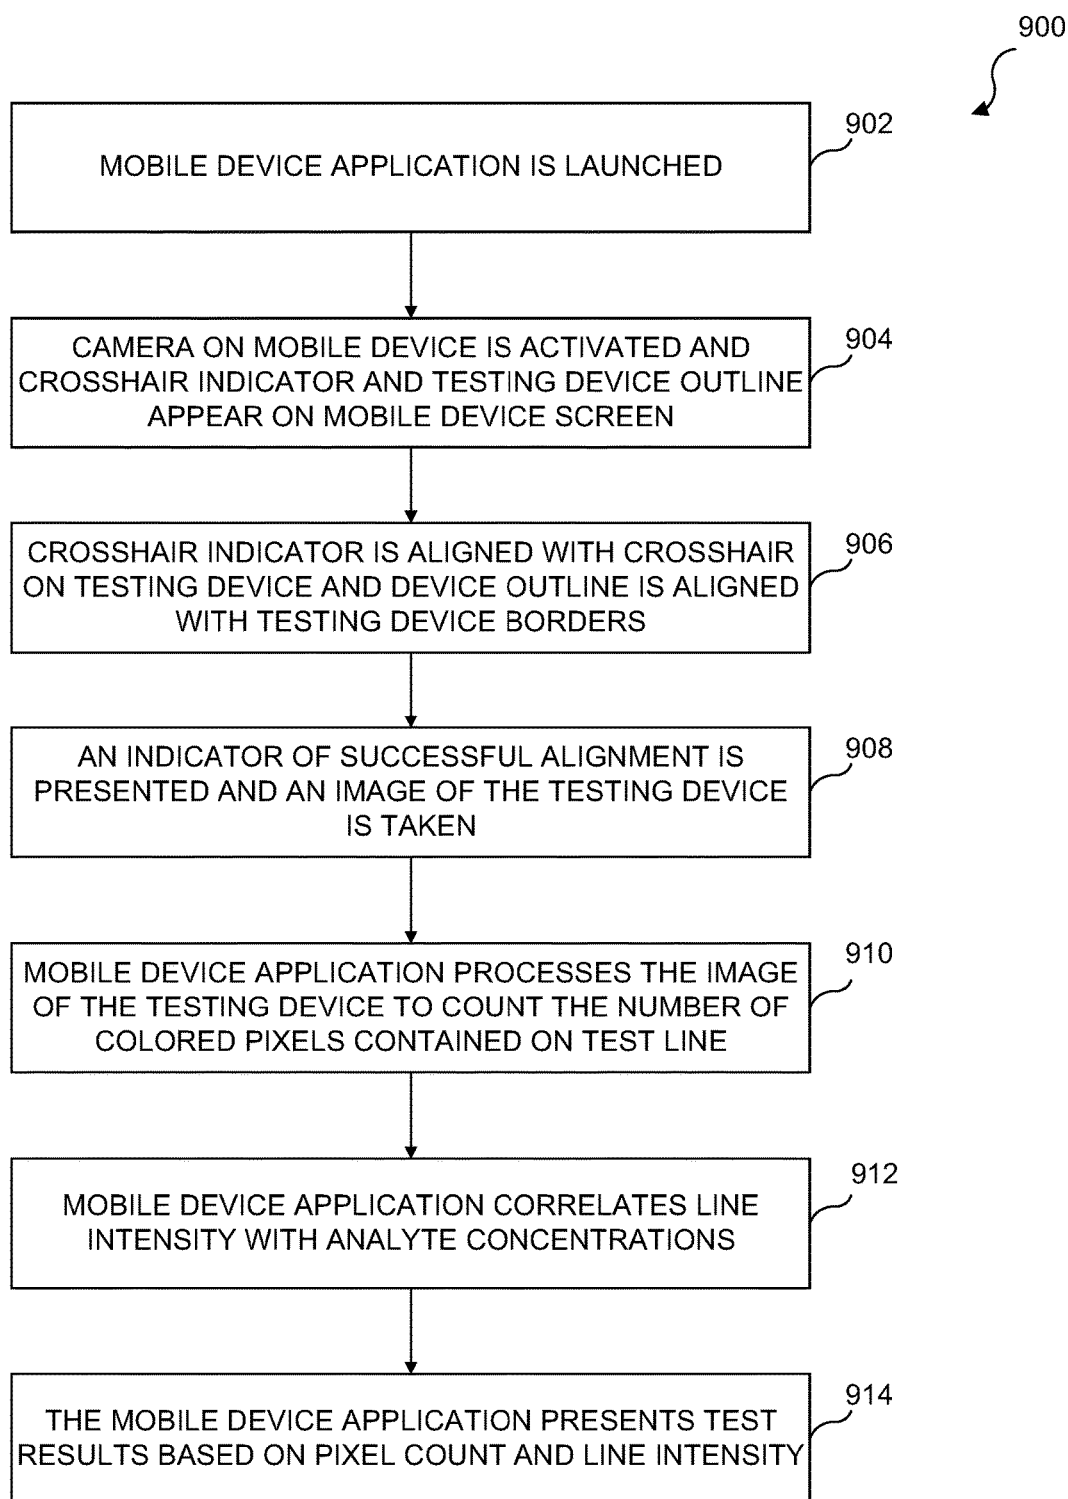


FIG. 9

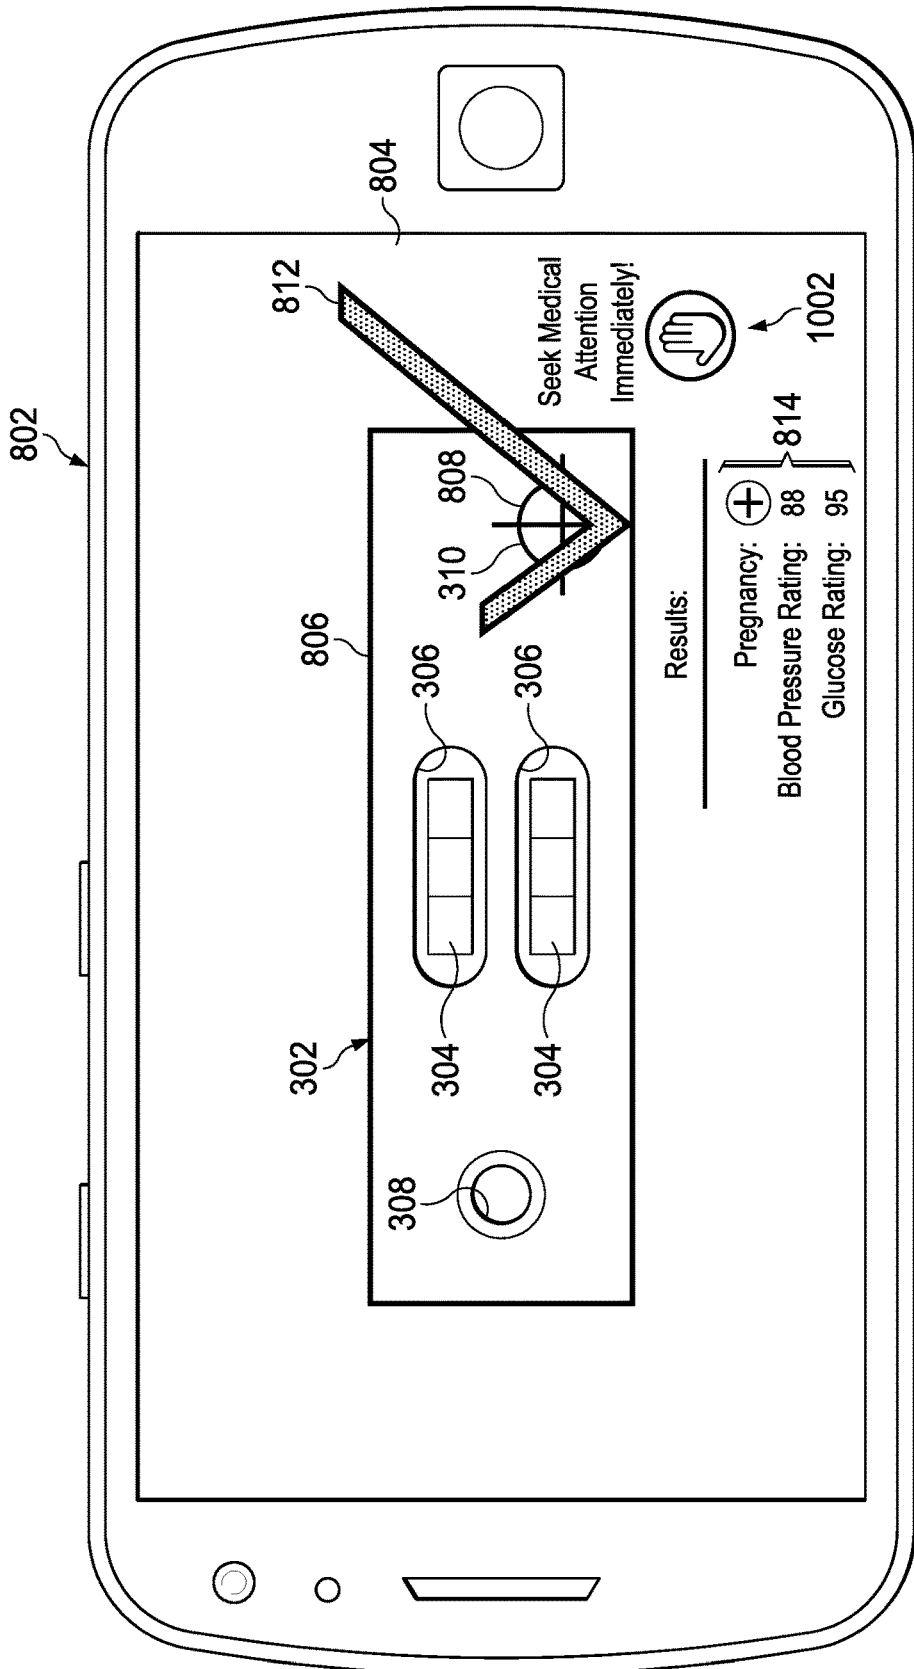


FIG. 10

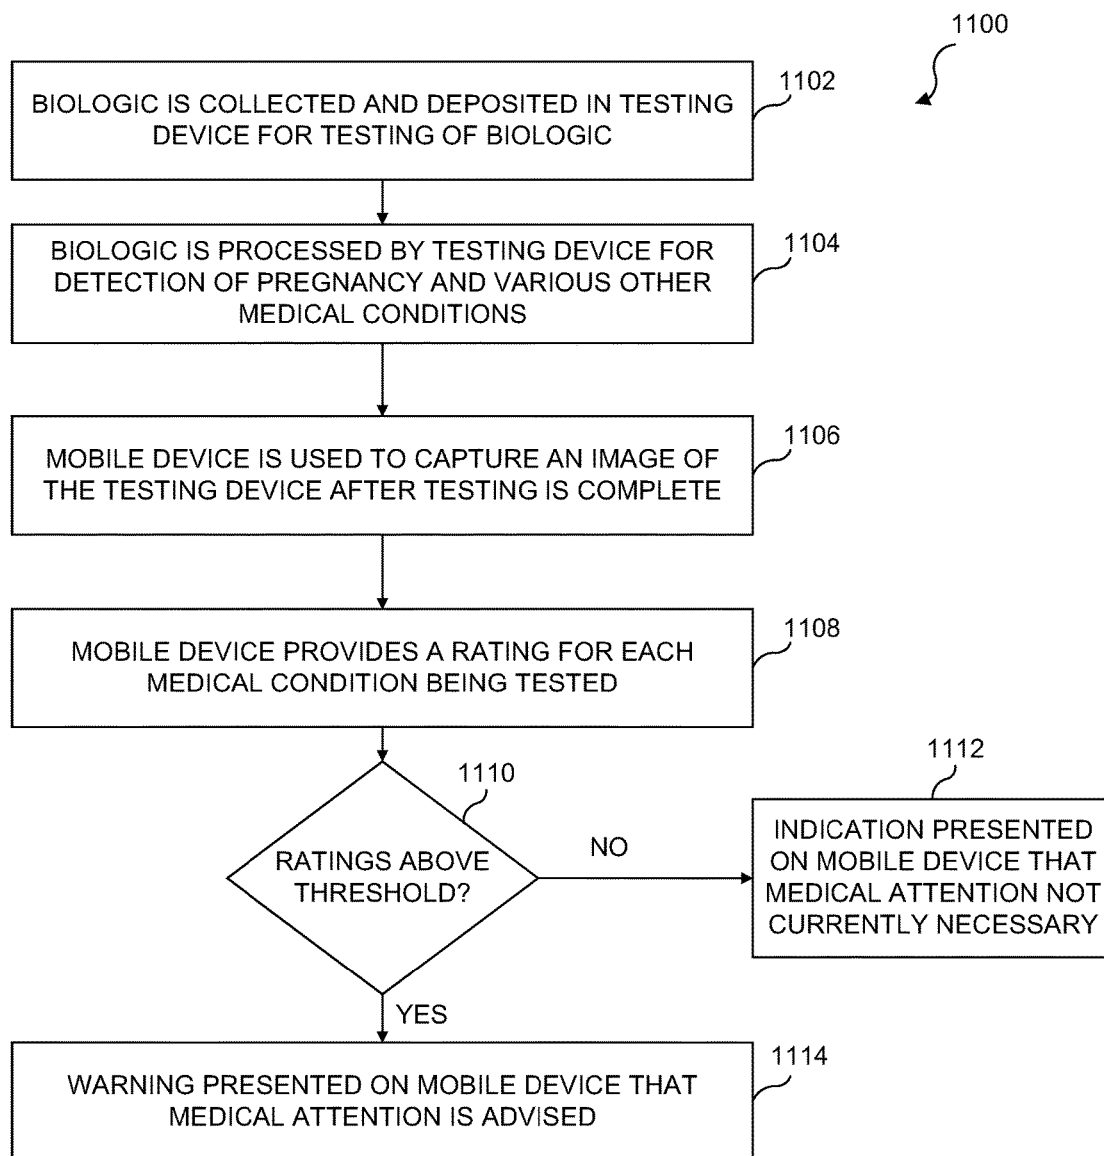


FIG. 11

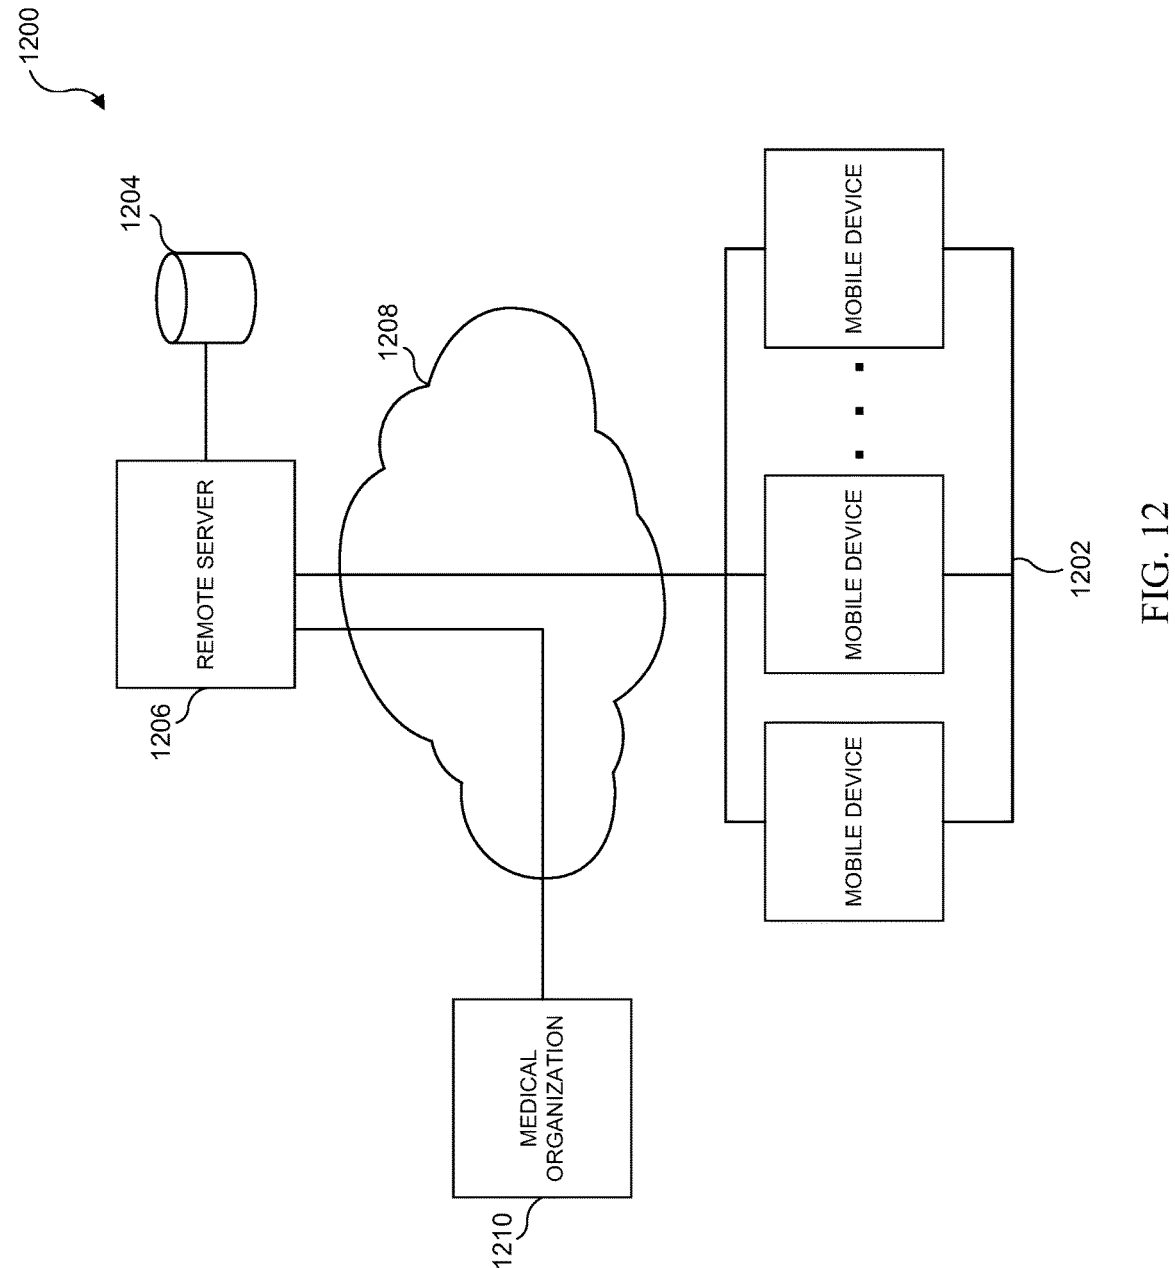


FIG. 12

1300

BIOLOGIC ID # 2402	
BIOLOGIC TYPE	BLOOD
PREGNANCY RATING	99
ZIKA INFECTION RATING	75
GLUCOSE RATING	10

1302

1304

1306

The diagram shows a table with a header row and four data rows. The header row is labeled 'BIOLOGIC ID # 2402' and is pointed to by callout 1302. The first two columns are labeled 'BIOLOGIC TYPE' and 'BLOOD', with the second column header pointed to by callout 1304. The data rows contain 'PREGNANCY RATING' (99), 'ZIKA INFECTION RATING' (75), and 'GLUCOSE RATING' (10). A bracket on the right side of the last three rows is pointed to by callout 1306. A separate callout 1300 points to the top right of the table area.

FIG. 13

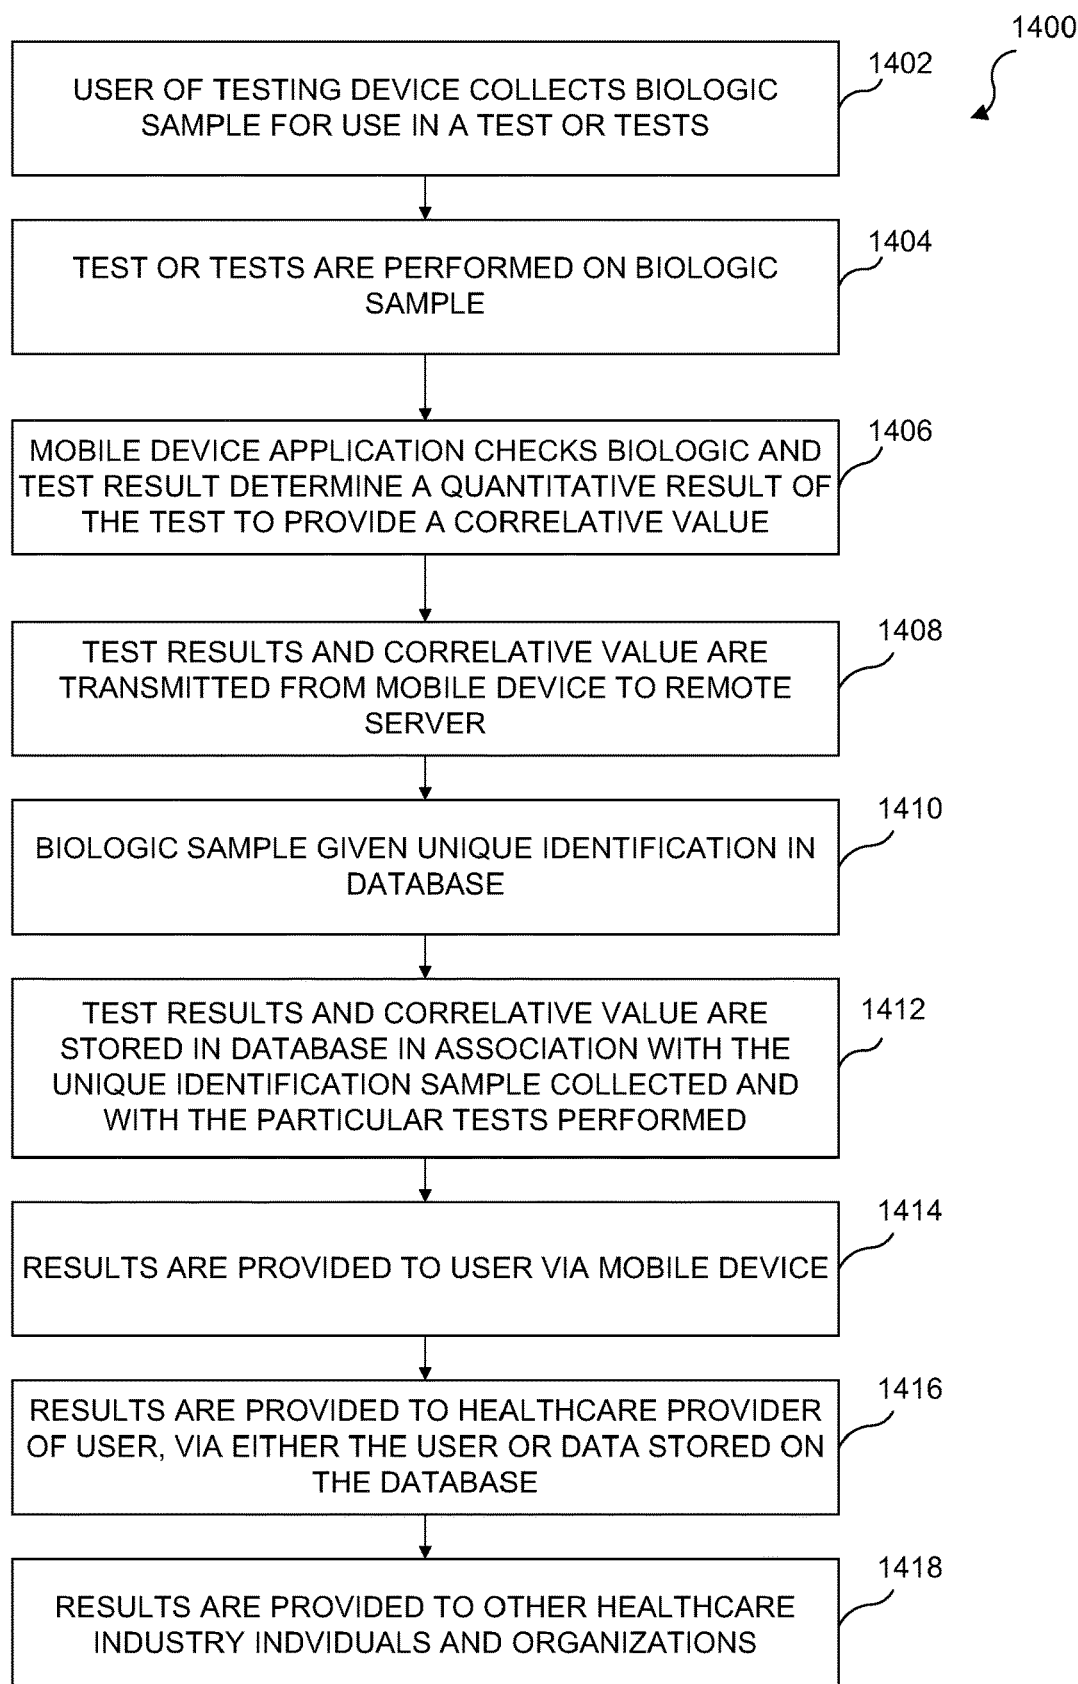
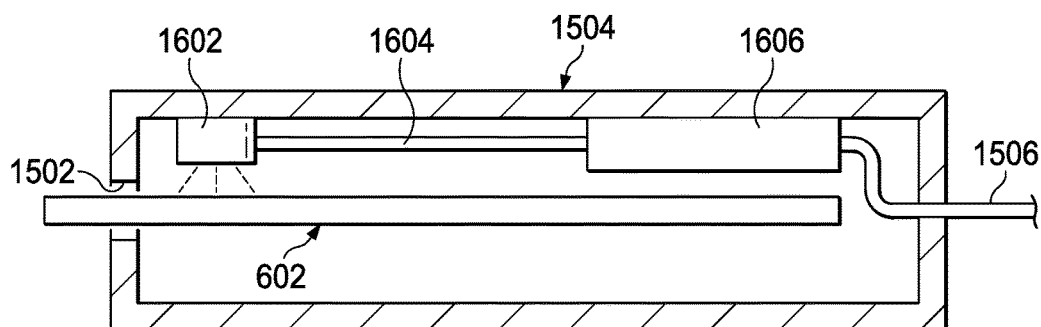
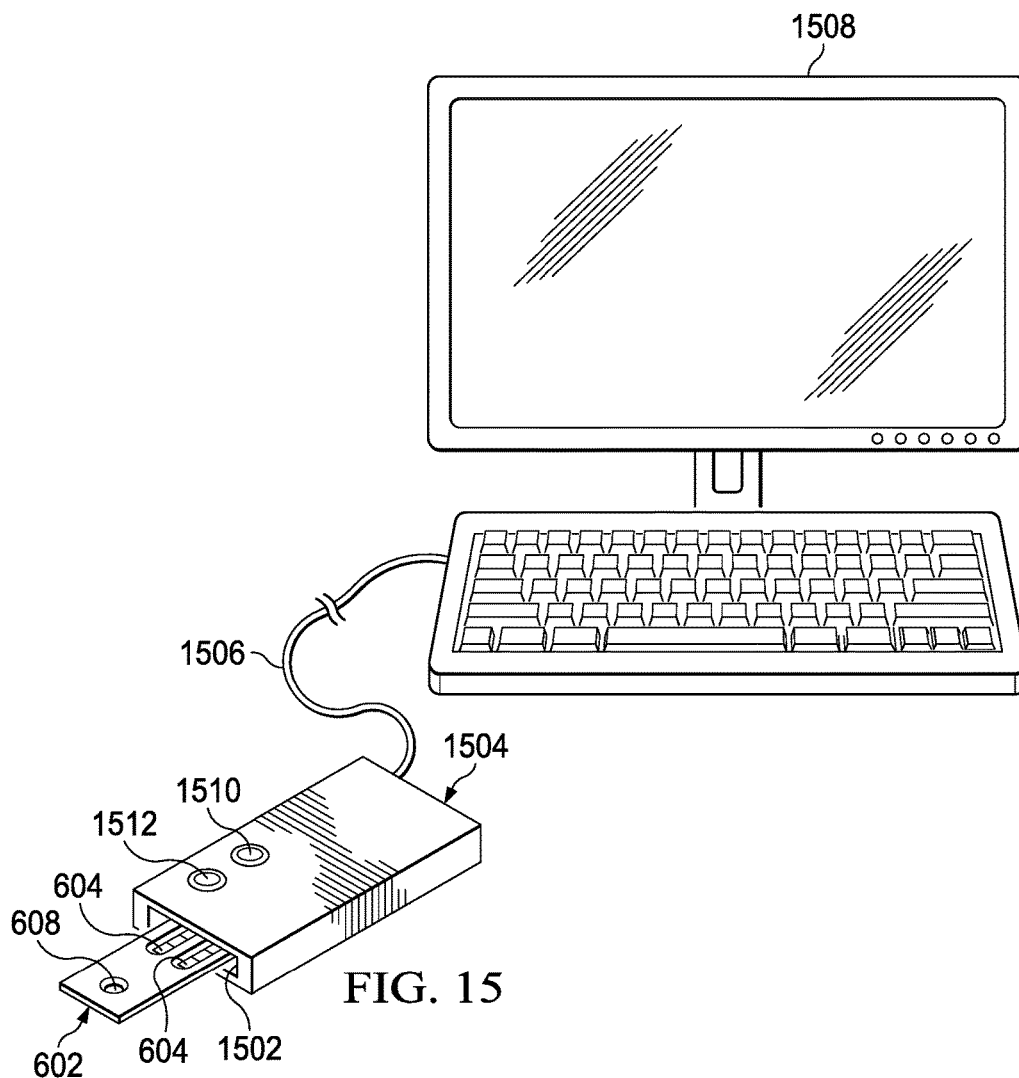


FIG. 14



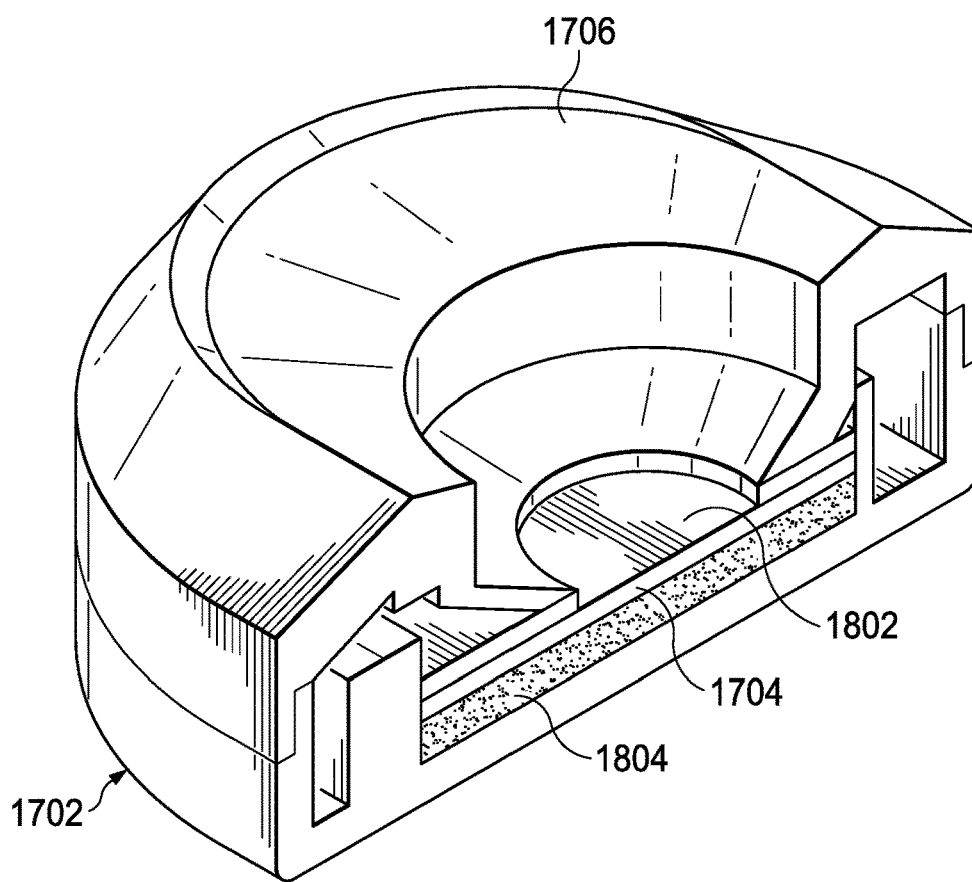
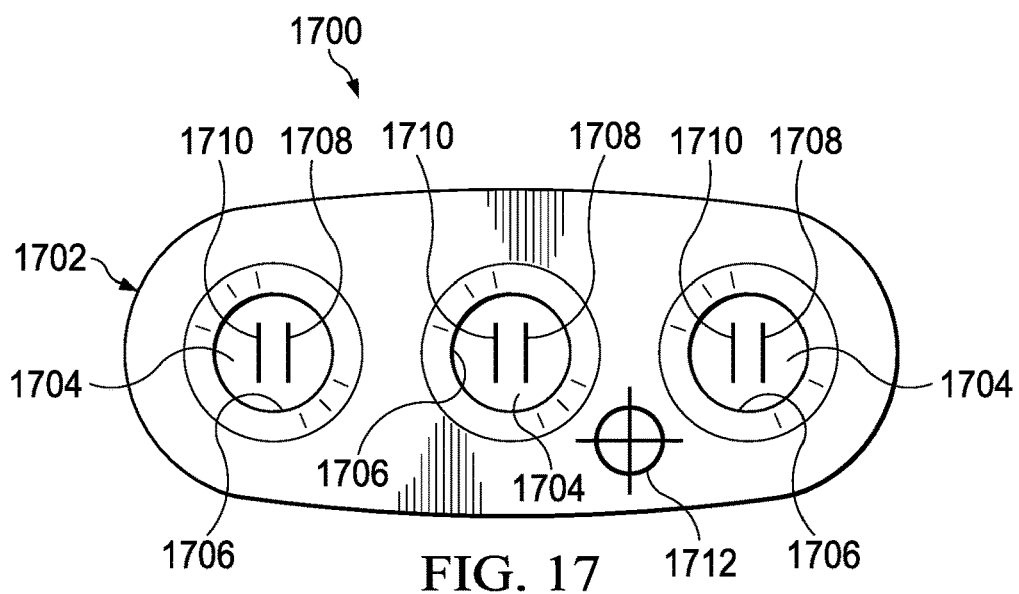


FIG. 18



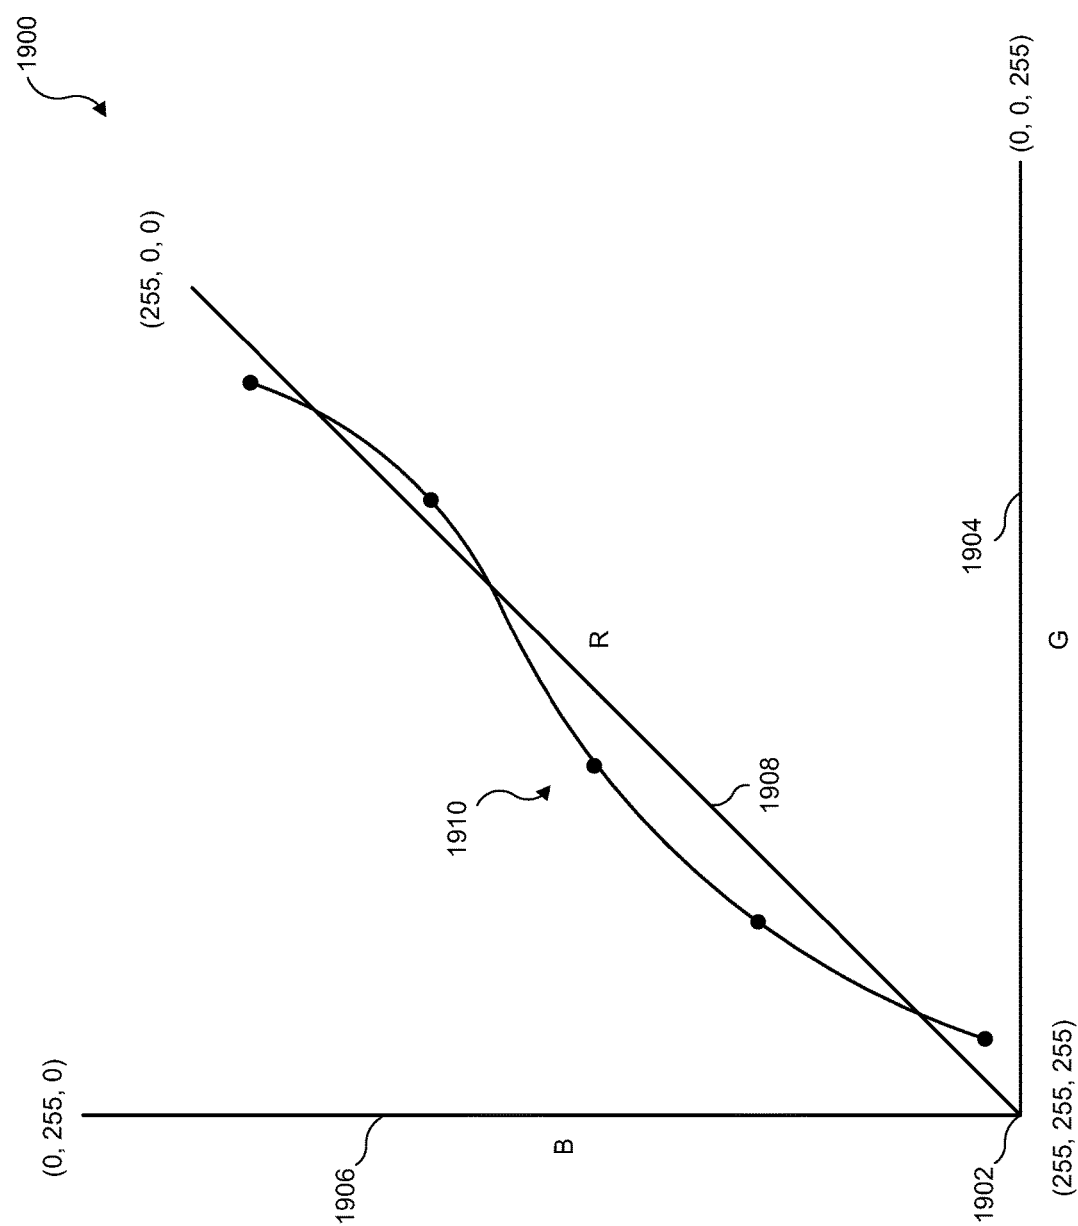


FIG. 19

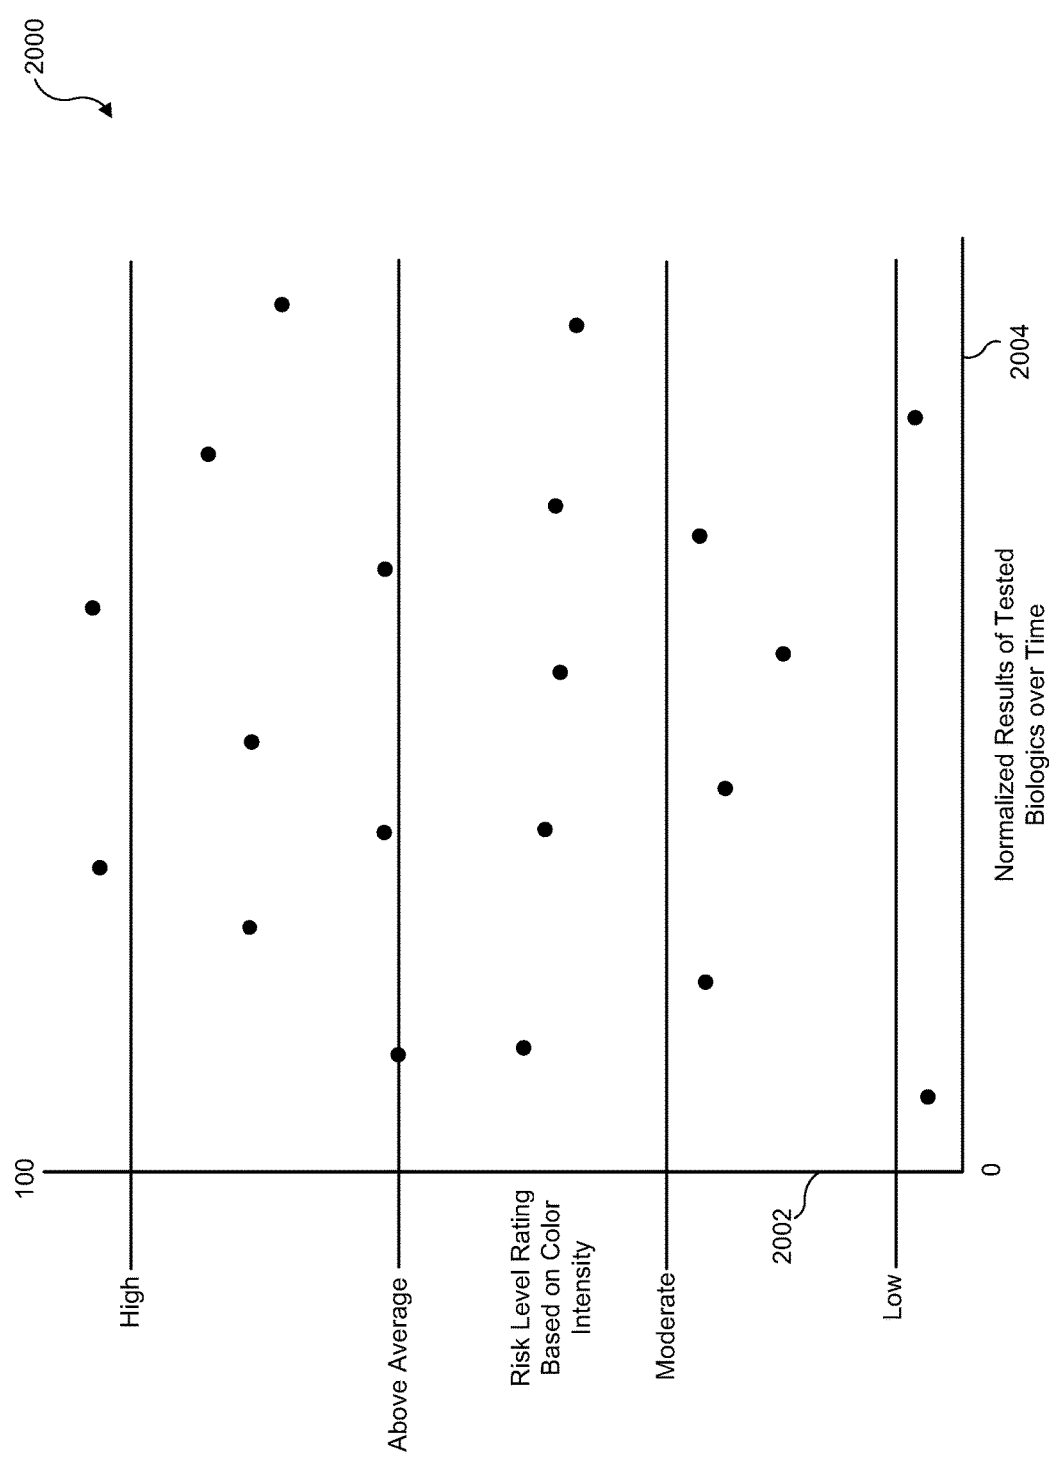


FIG. 20

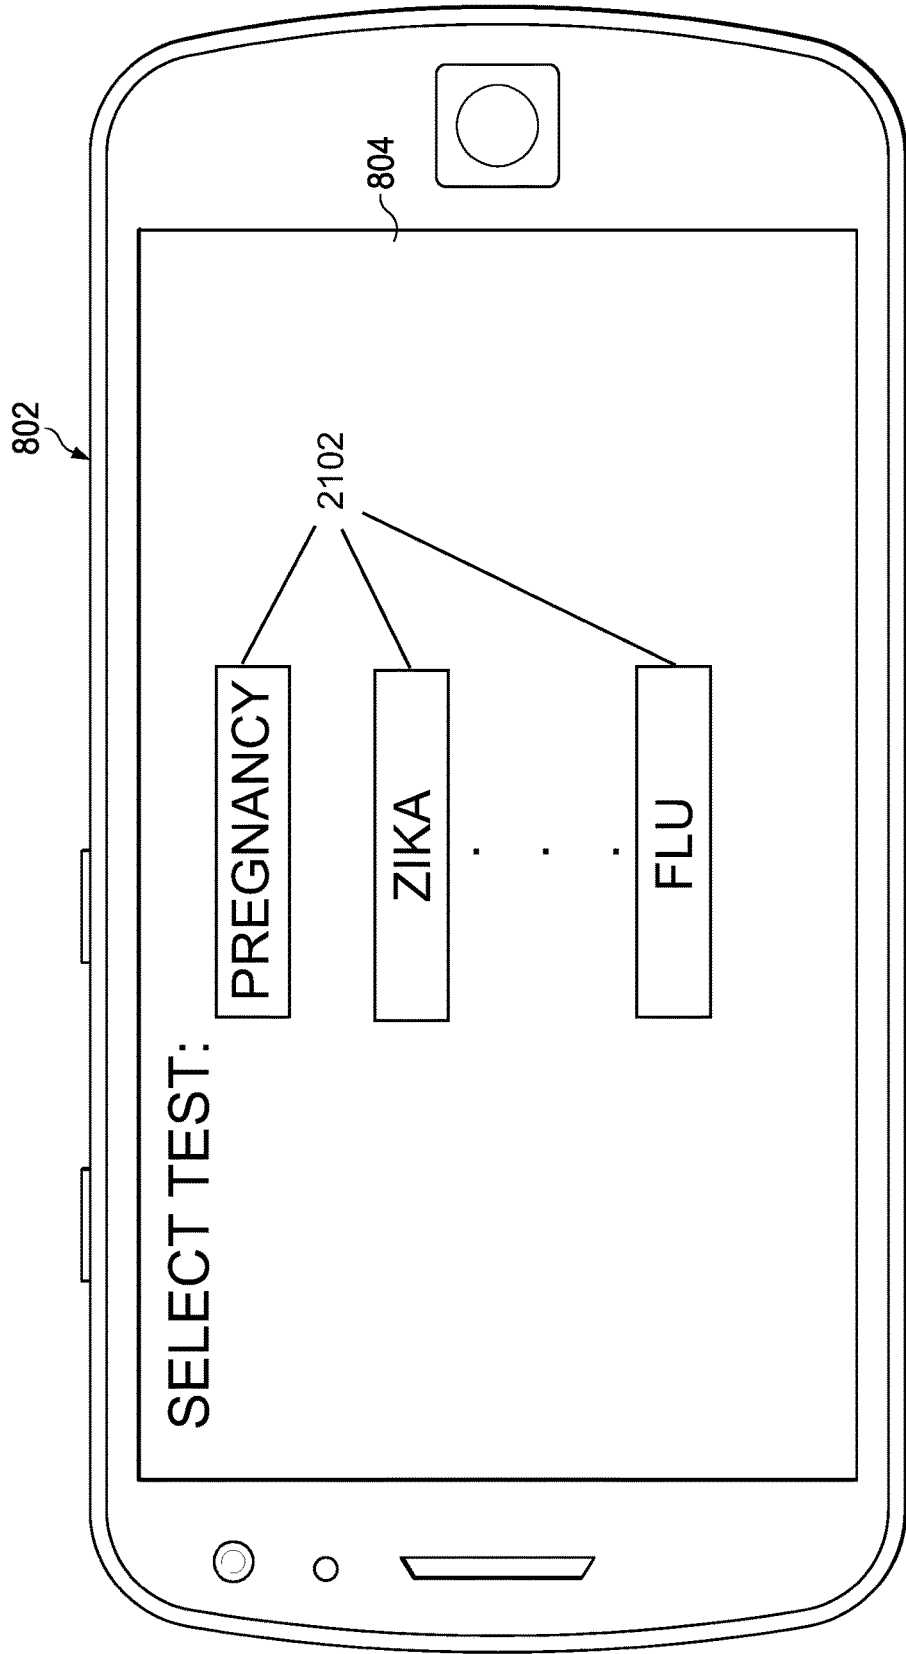


FIG. 21

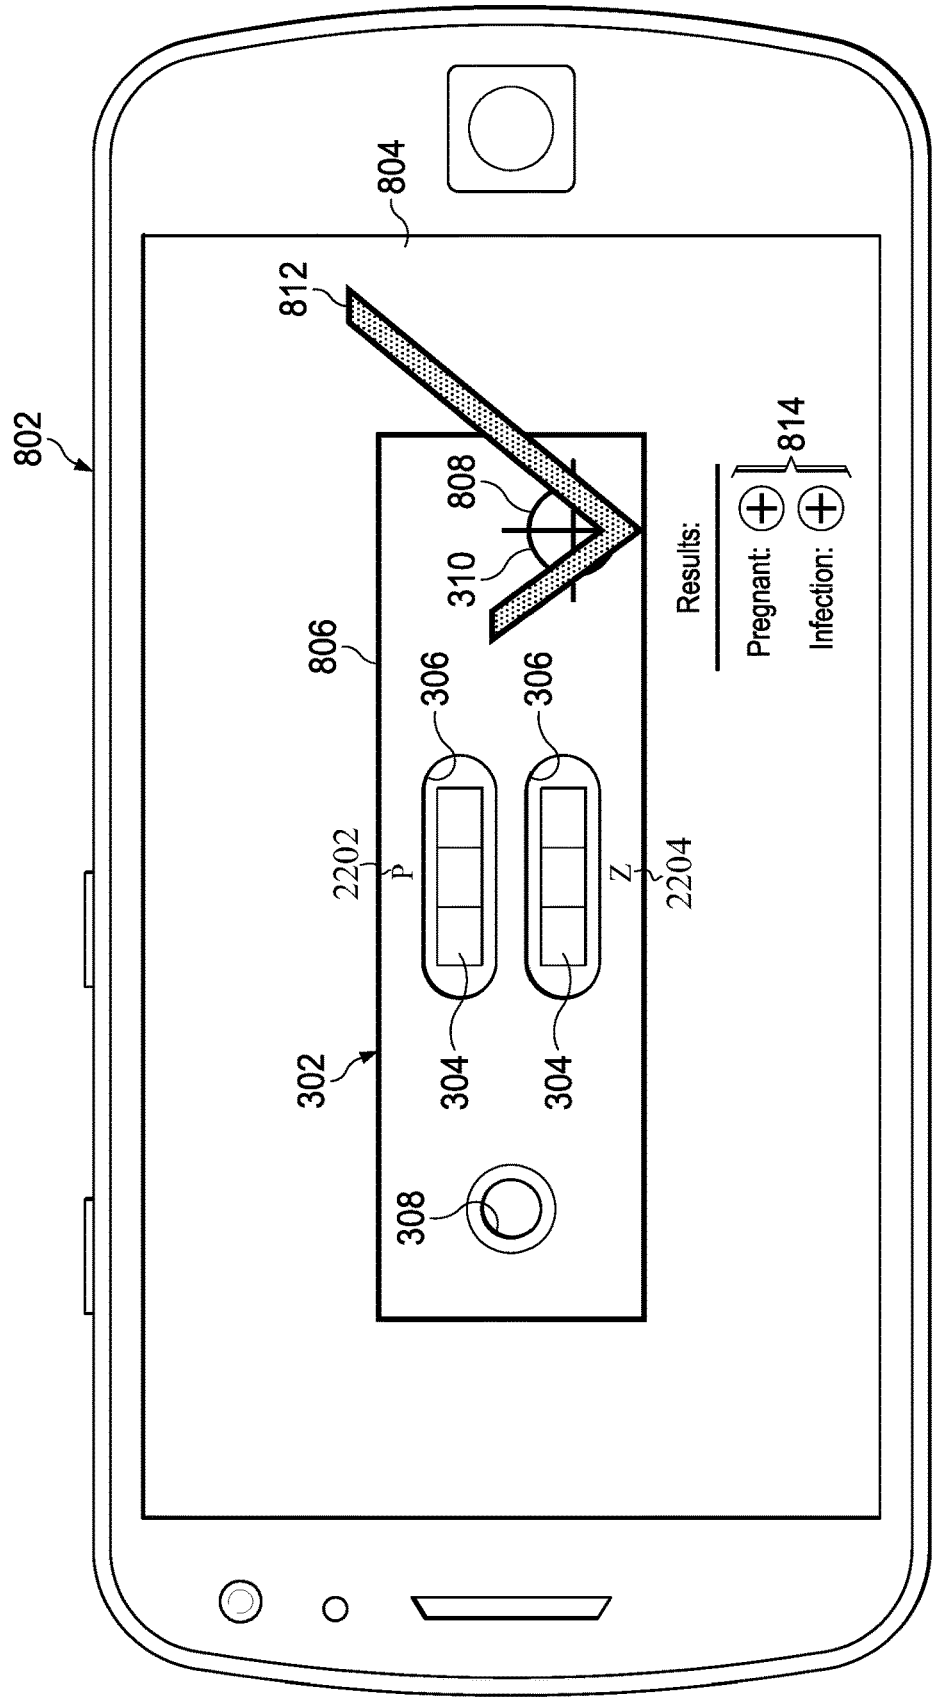


FIG. 22

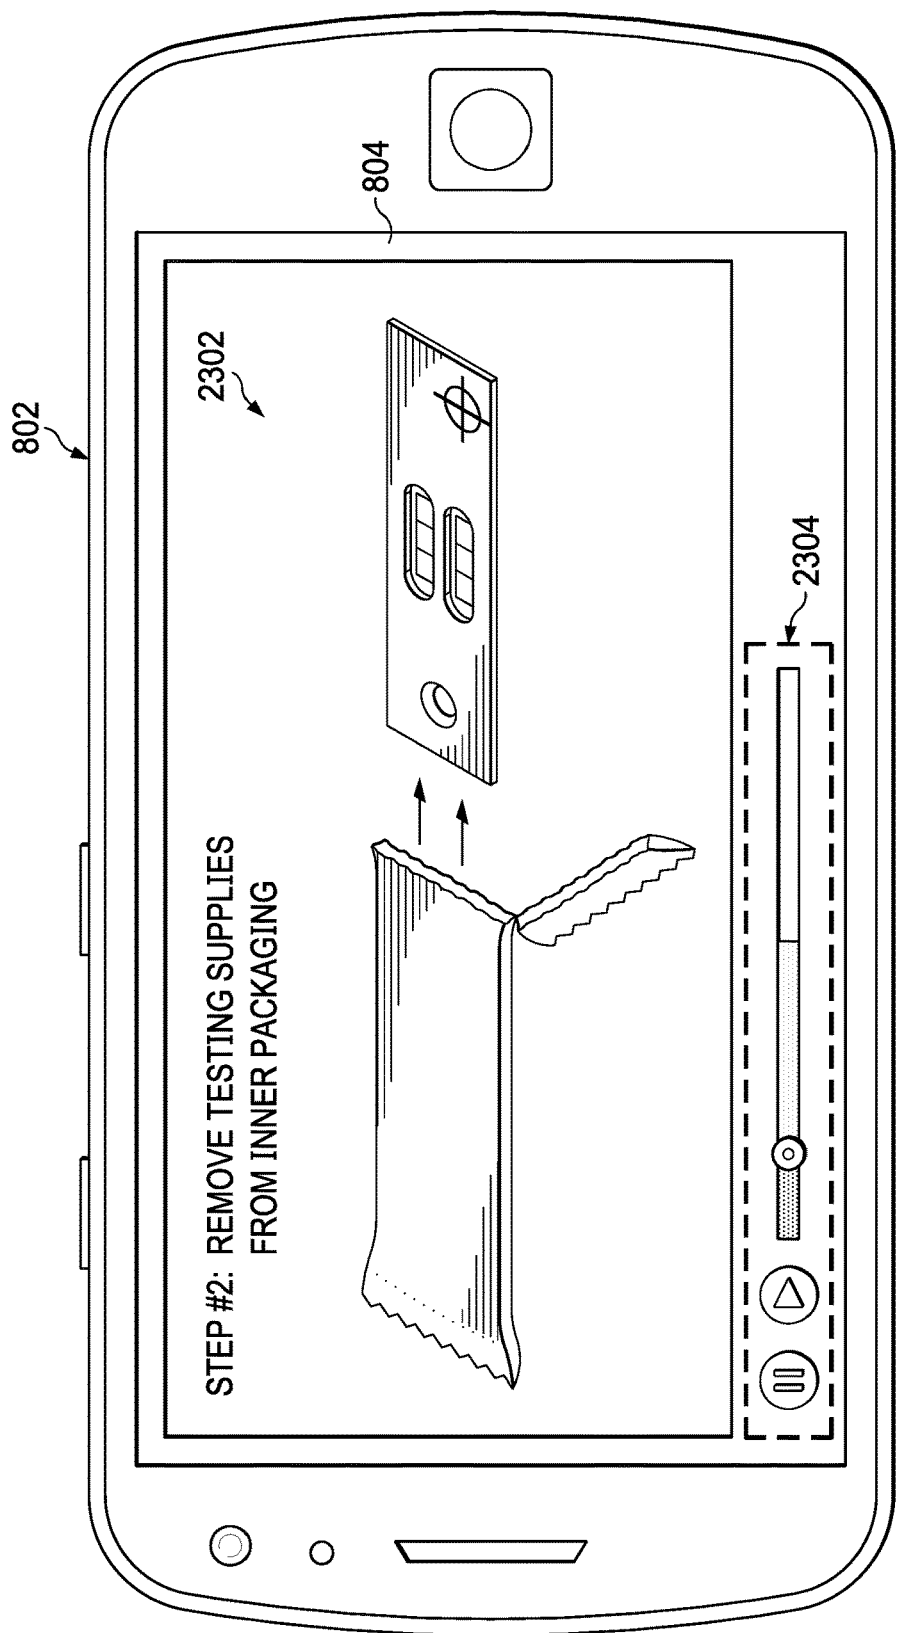


FIG. 23

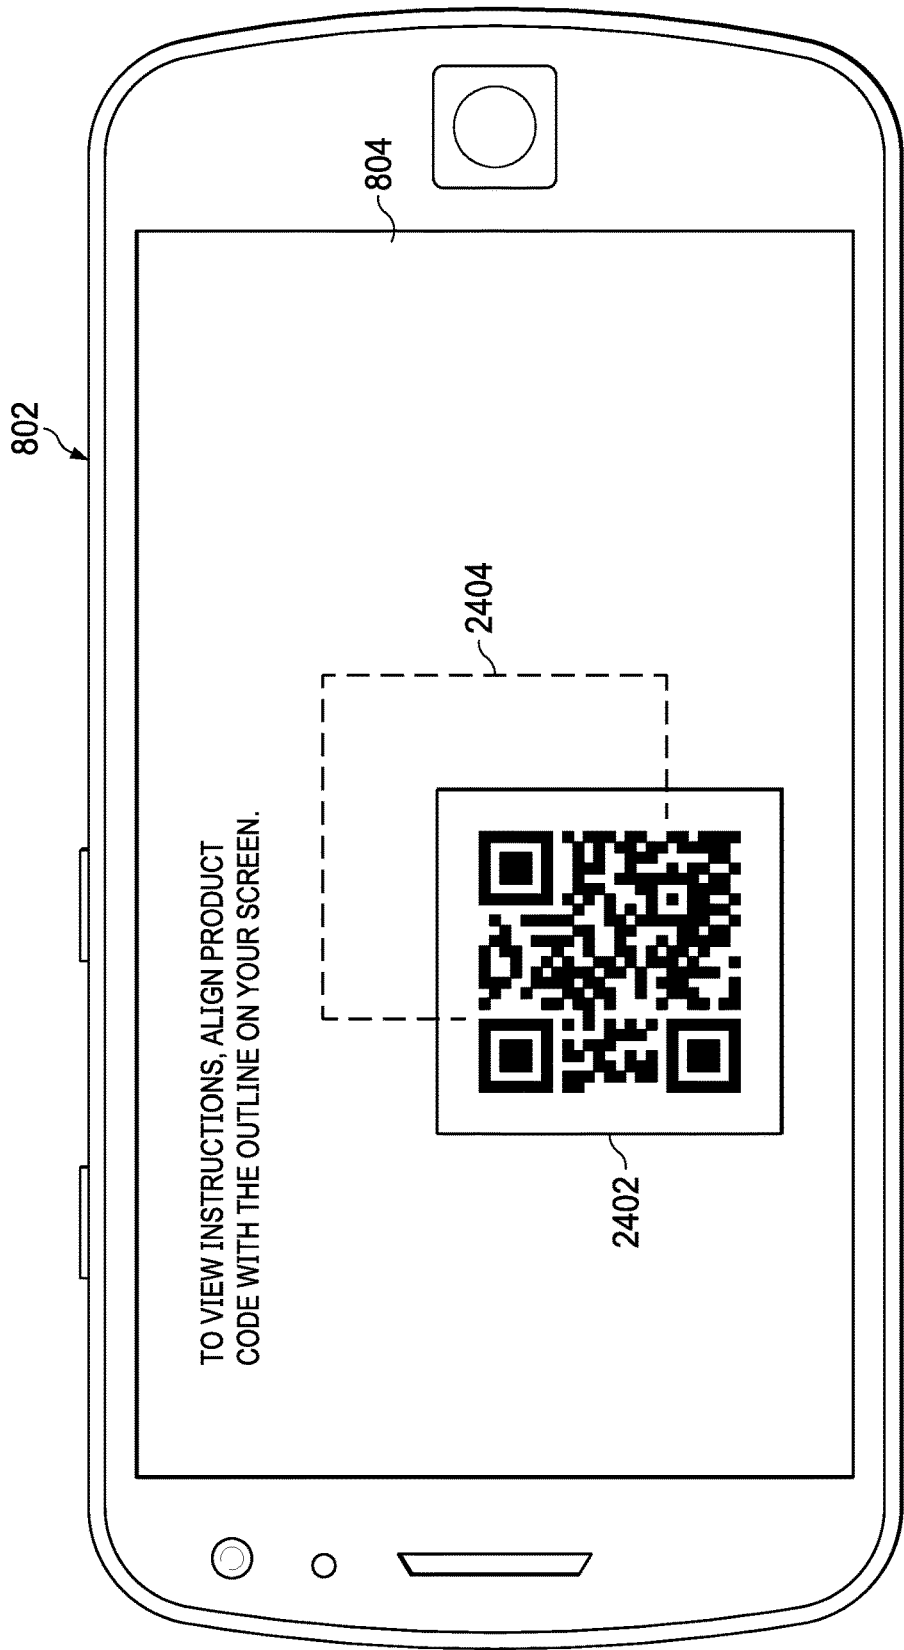


FIG. 24

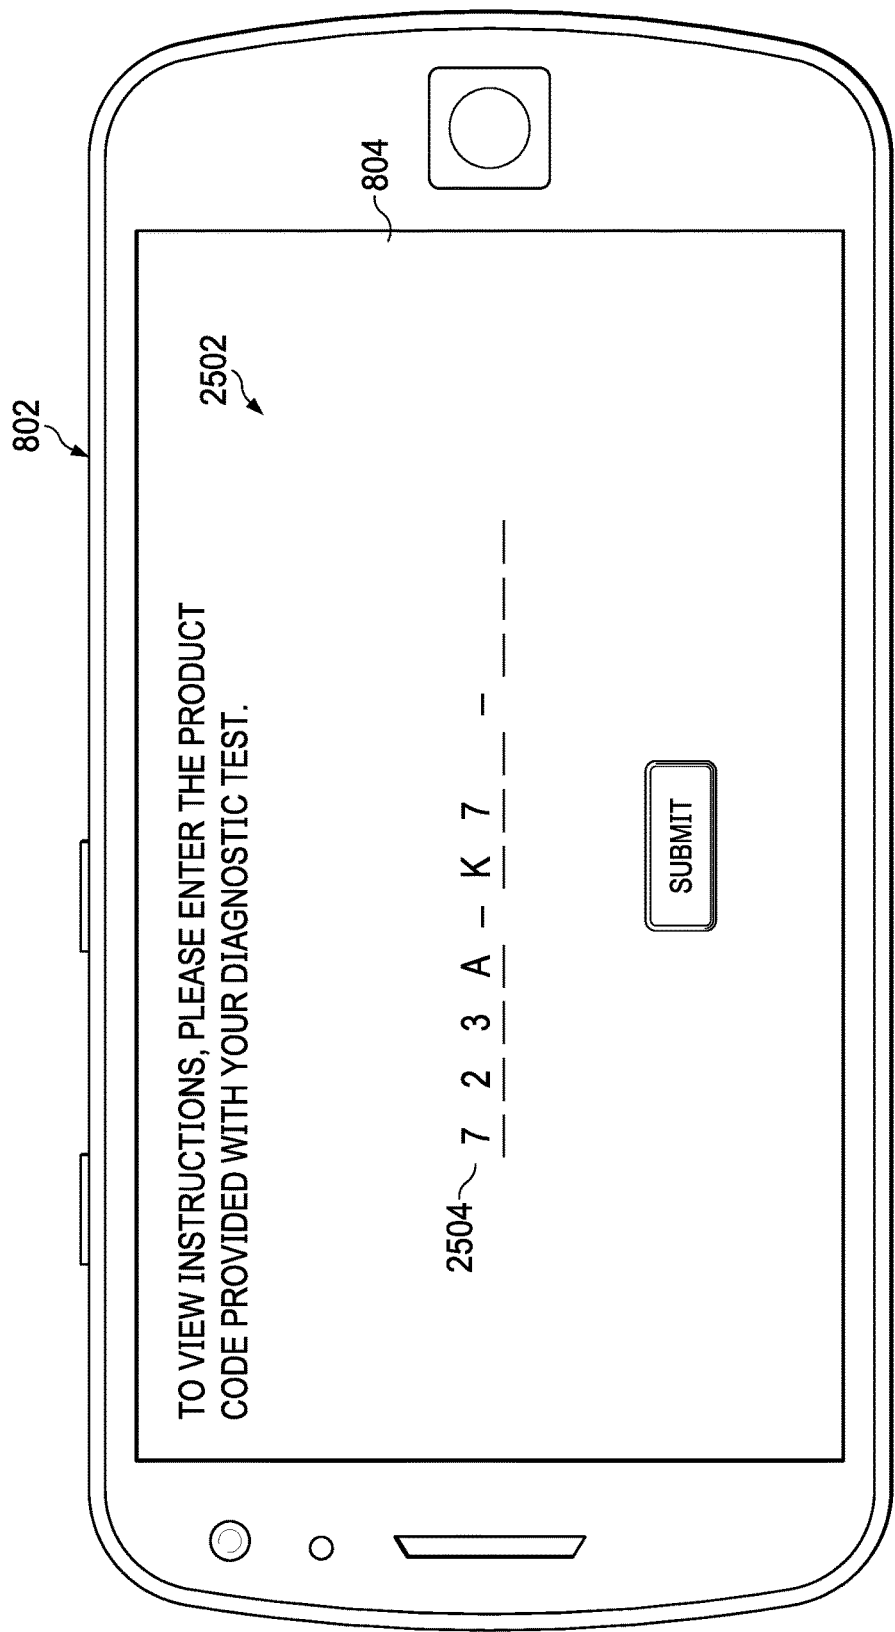


FIG. 25

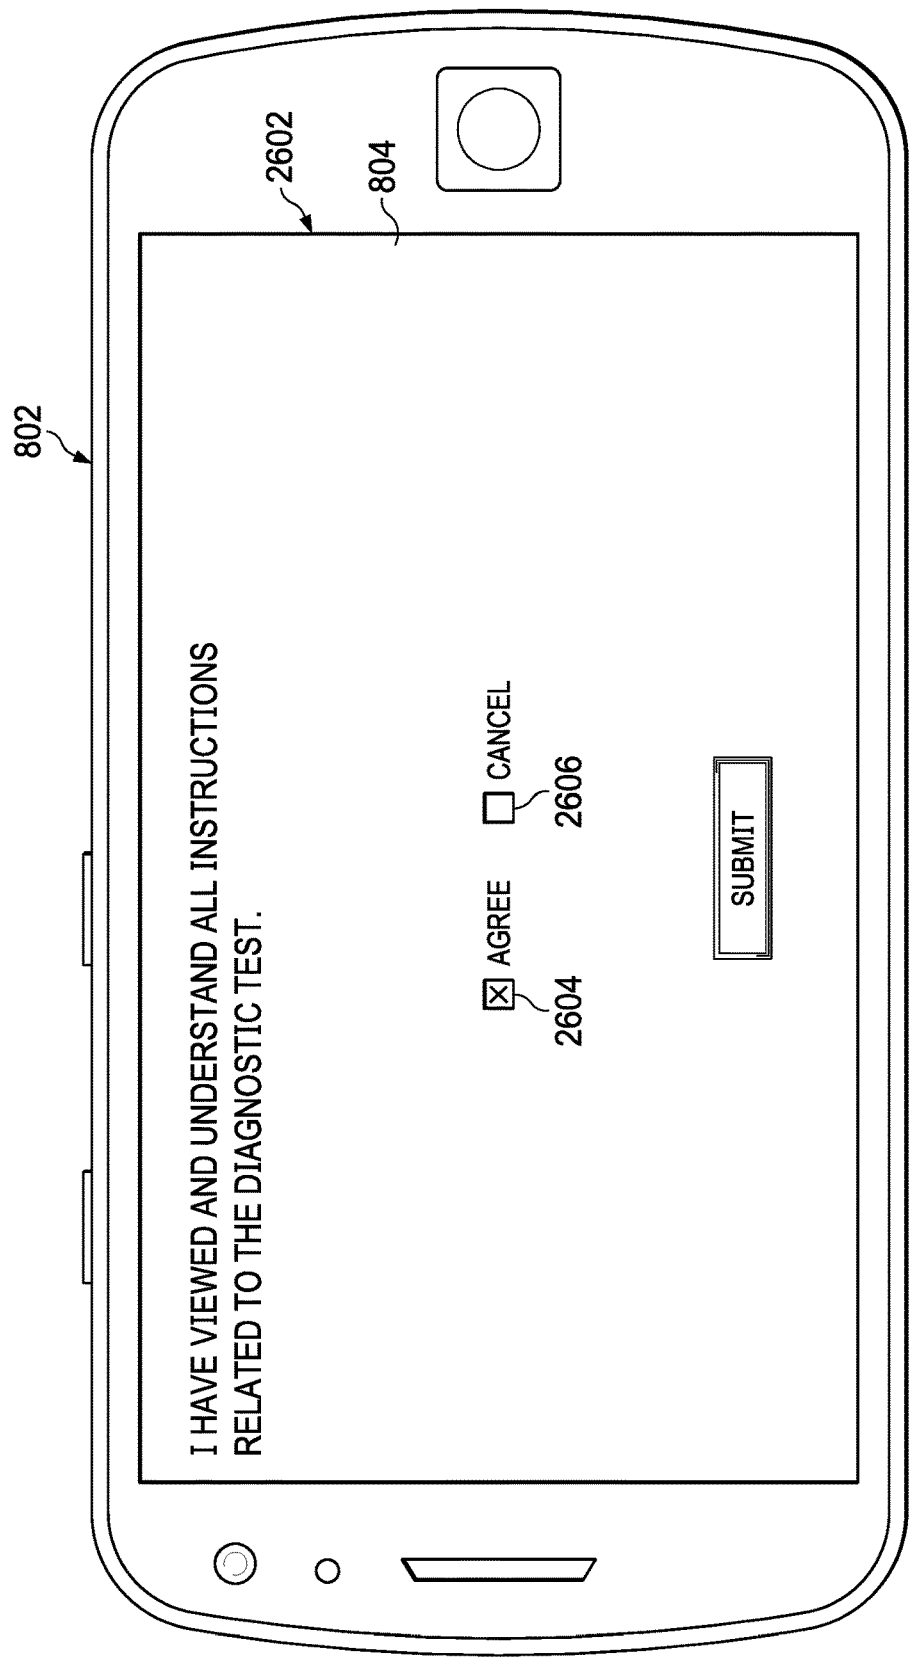


FIG. 26



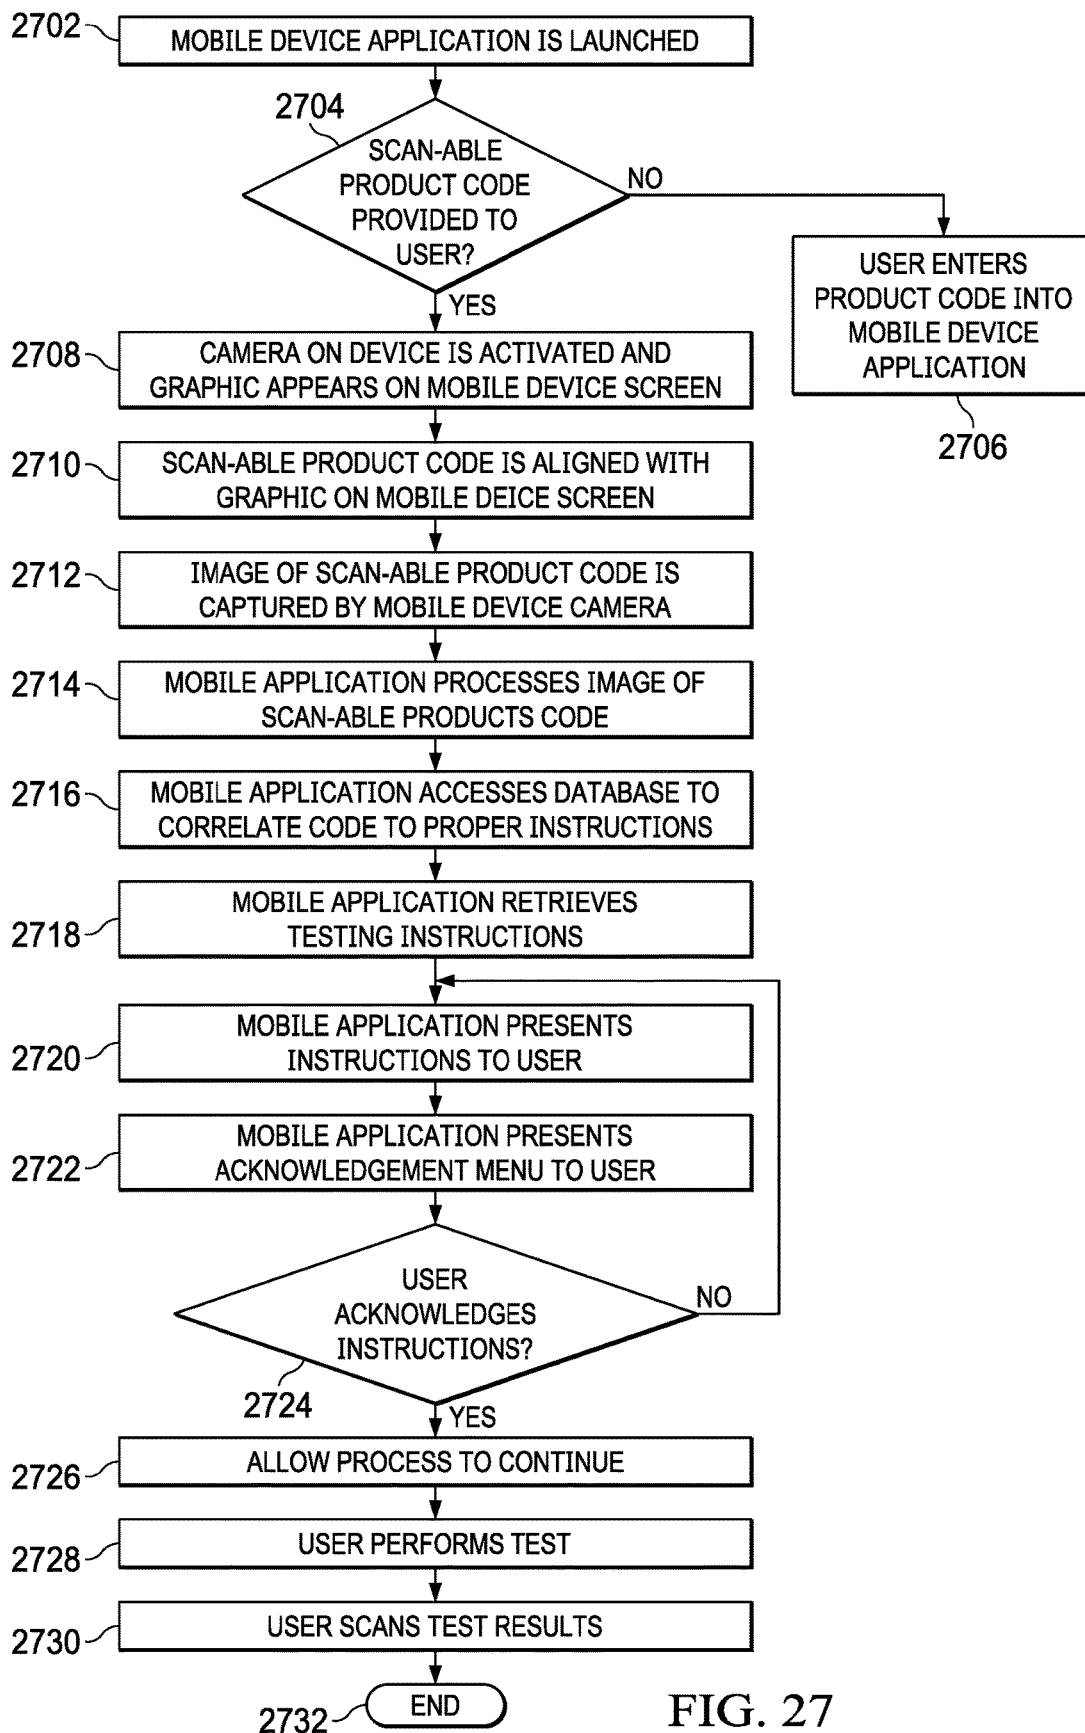


FIG. 27

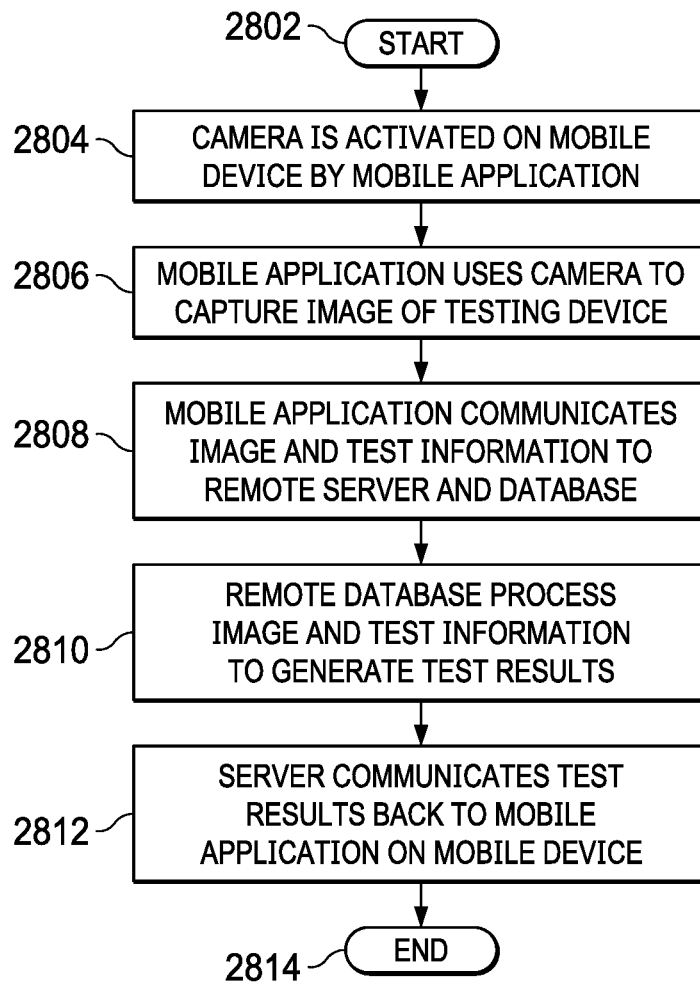


FIG. 28

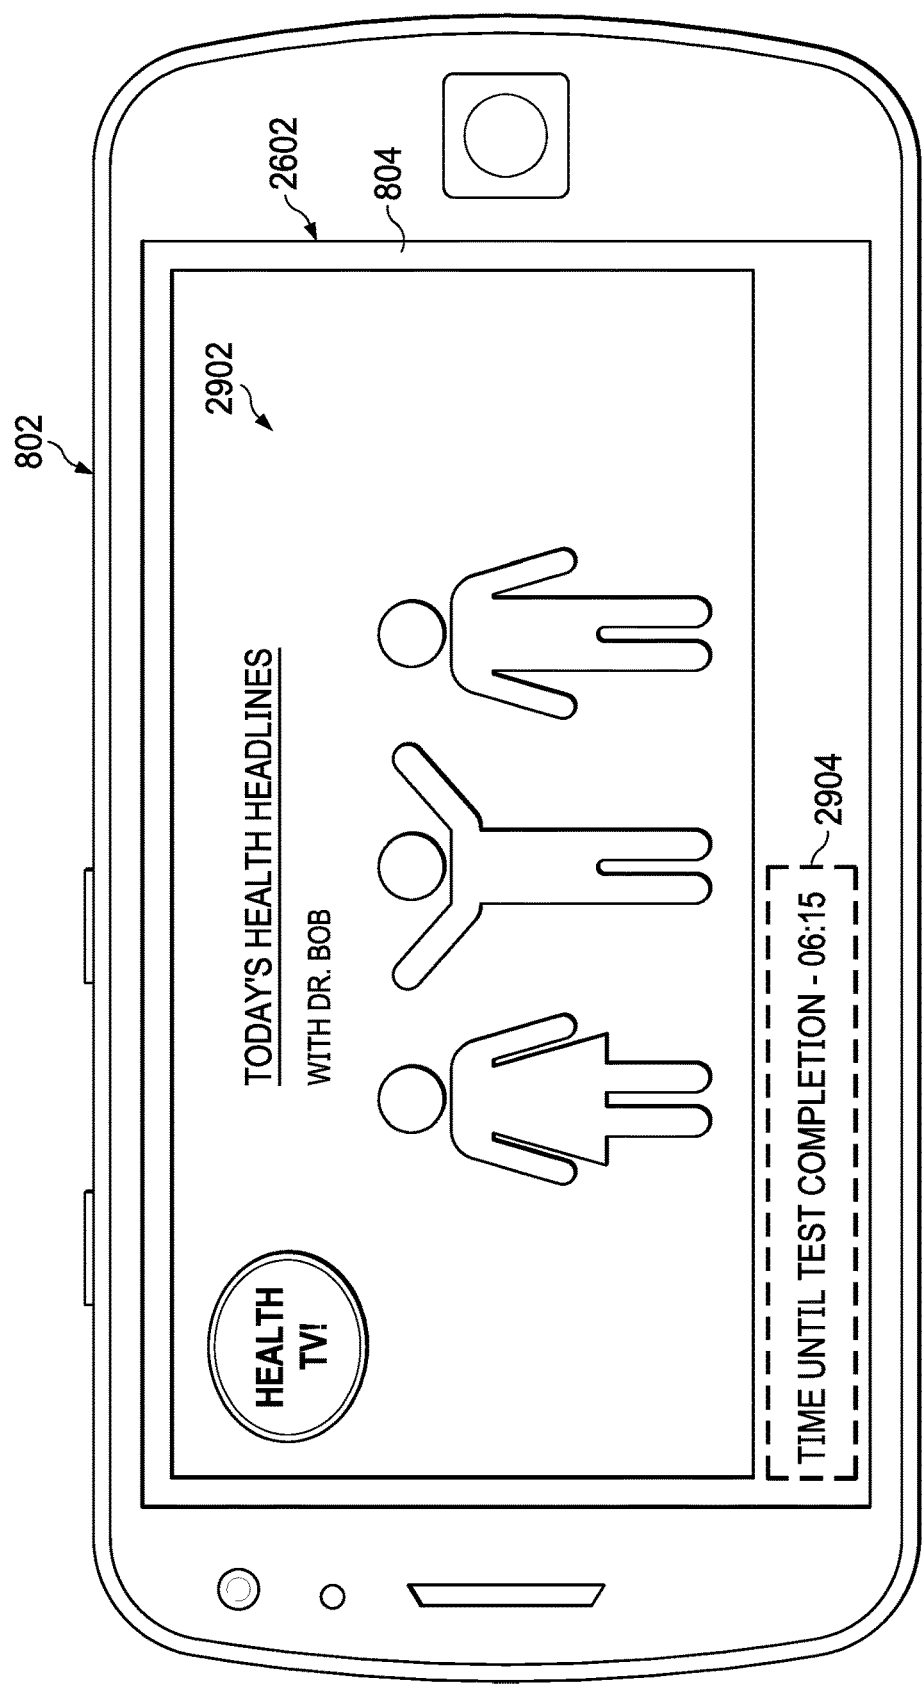


FIG. 29

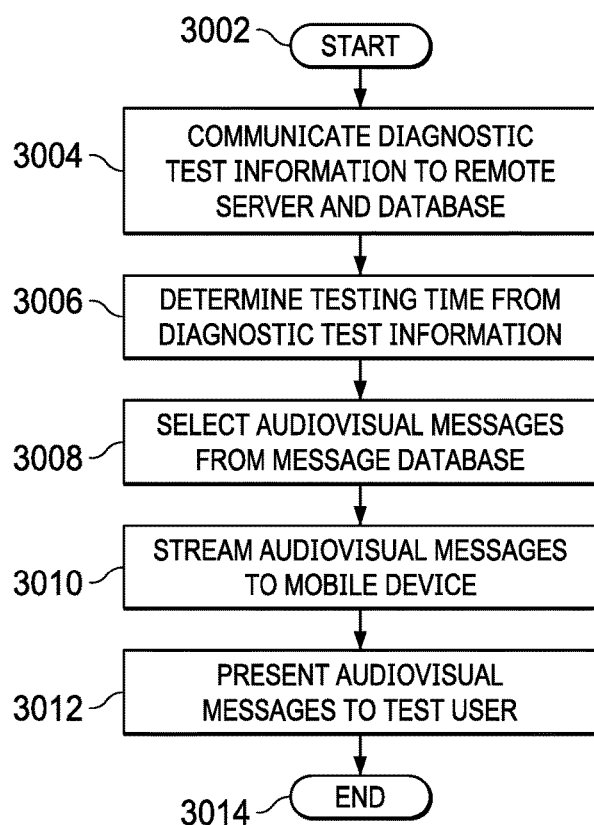


FIG. 30

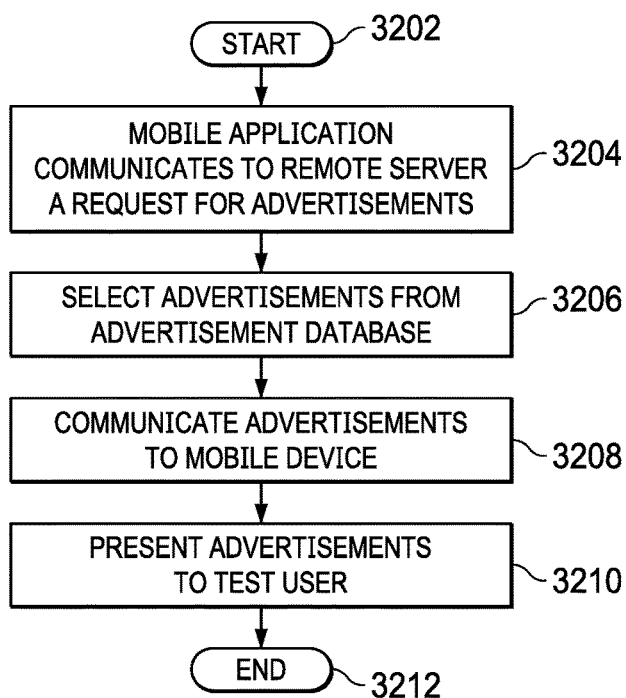


FIG. 32

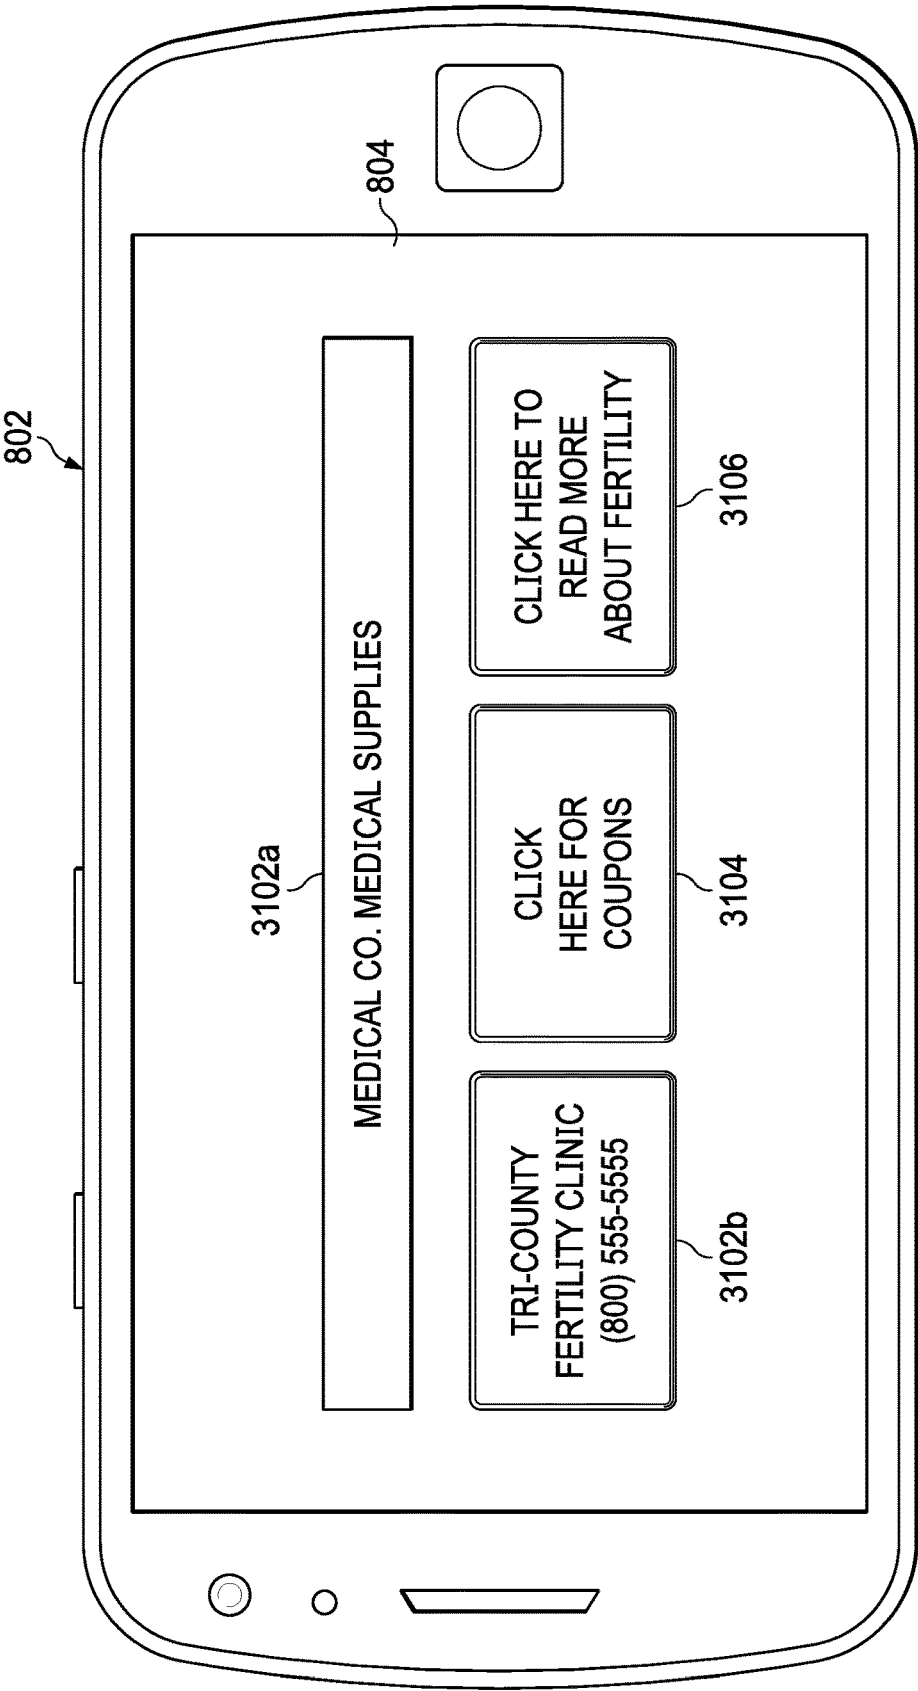


FIG. 31

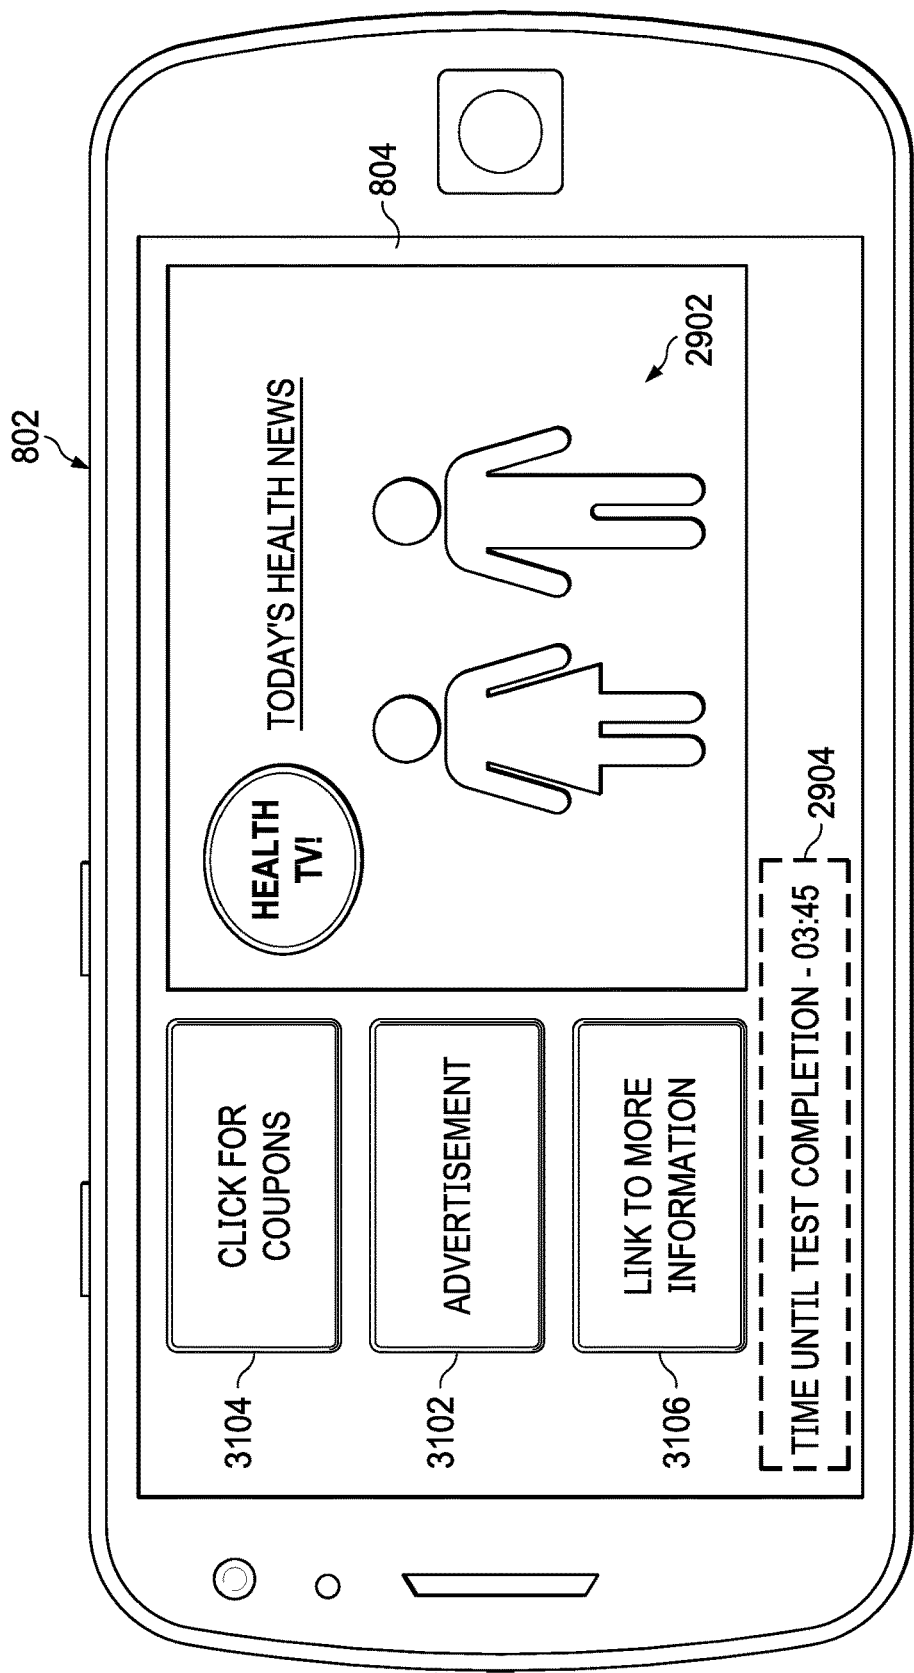


FIG. 33

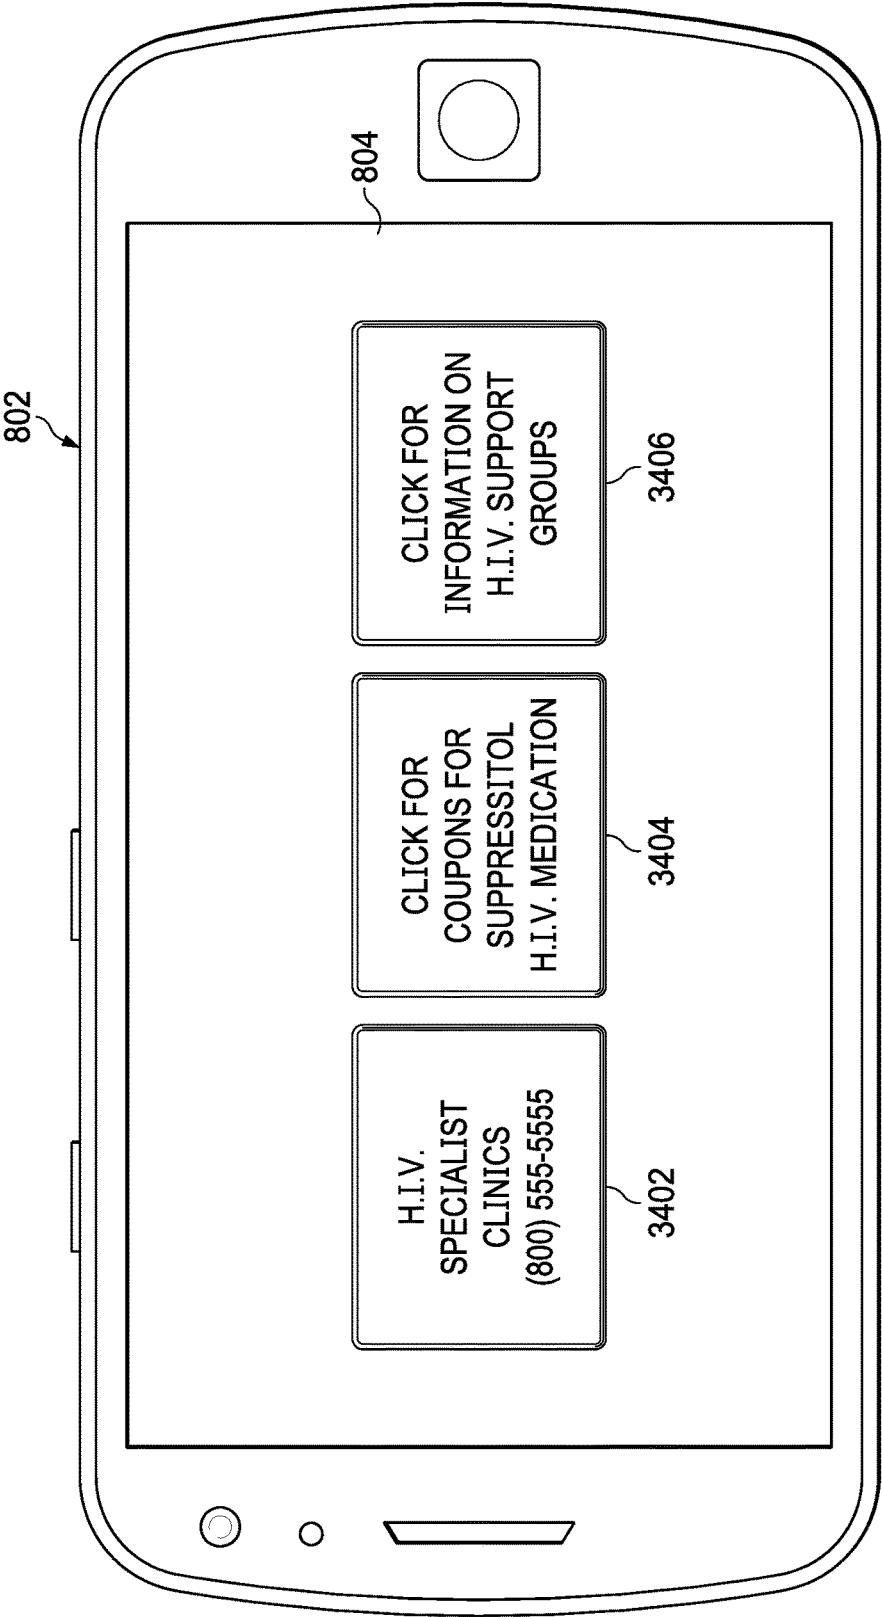


FIG. 34

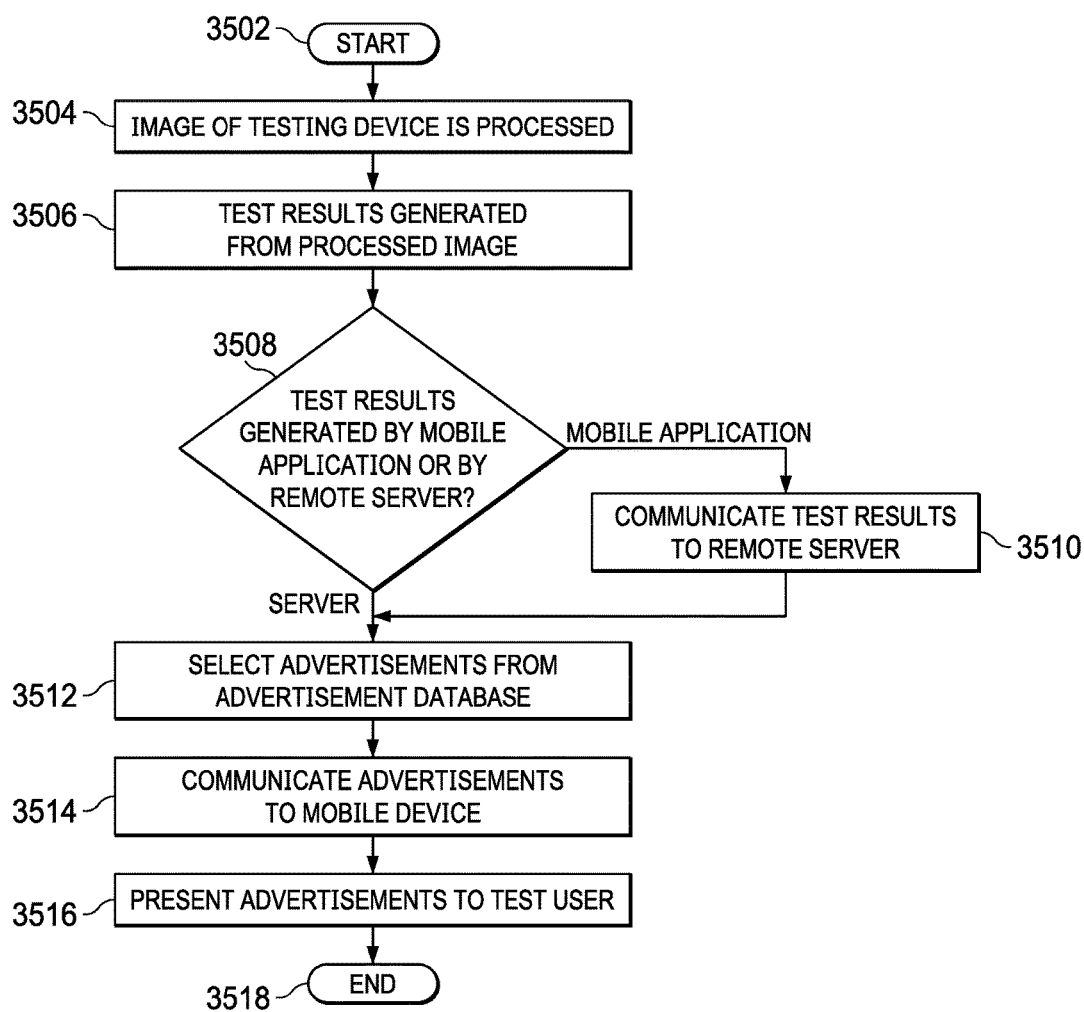


FIG. 35



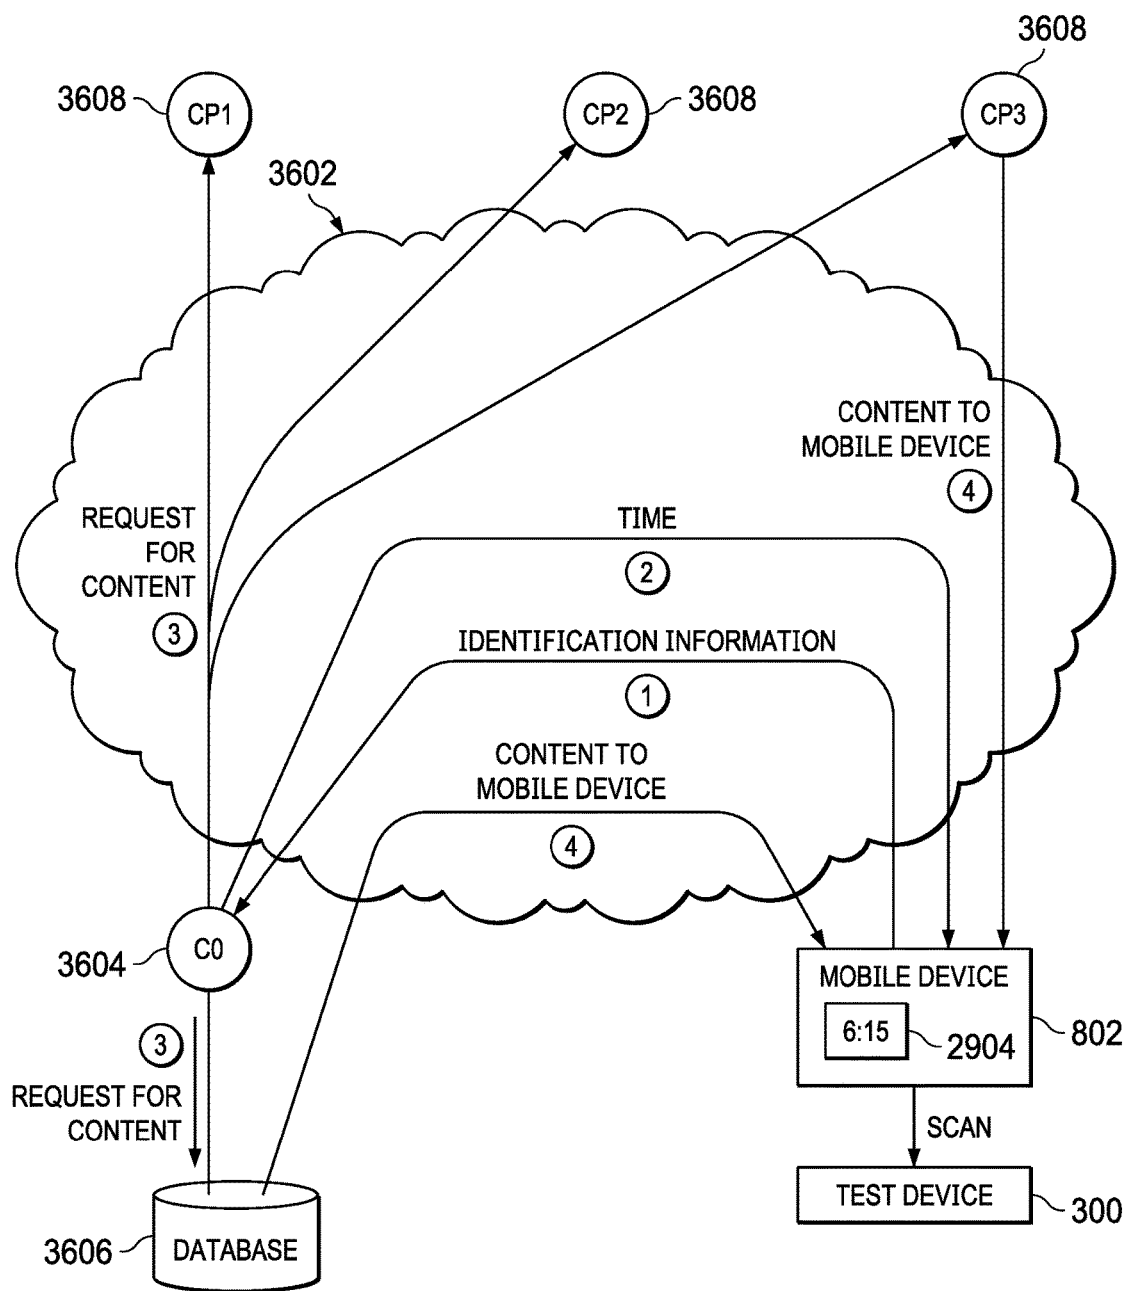


FIG. 36

3702a		3702c	
CODE	CONTENT	CODE	CONTENT
XXXX	MESSAGE A	$T_0 - T_1$	MESSAGE Q
YYYY	MESSAGE B	$T_1 - T_2$	MESSAGE X
ZZZZ	MESSAGE C	$T_2 - T_3$	MESSAGE W
⋮	⋮	⋮	⋮

3702b			3702d	
CODE	RESULT	CONTENT	CONTENT PROVIDER	CONTENT
XXXX	P	MESSAGE R	CP1	MESSAGE A,B,C
	N	MESSAGE T		
YYYY	P	MESSAGE Q	CP2	MESSAGE X,Y,Z
	N	MESSAGE M		
ZZZZ	P	MESSAGE F	CP3	MESSAGE L,M,N
	N	MESSAGE P		
⋮	⋮	⋮	⋮	⋮

FIG. 37

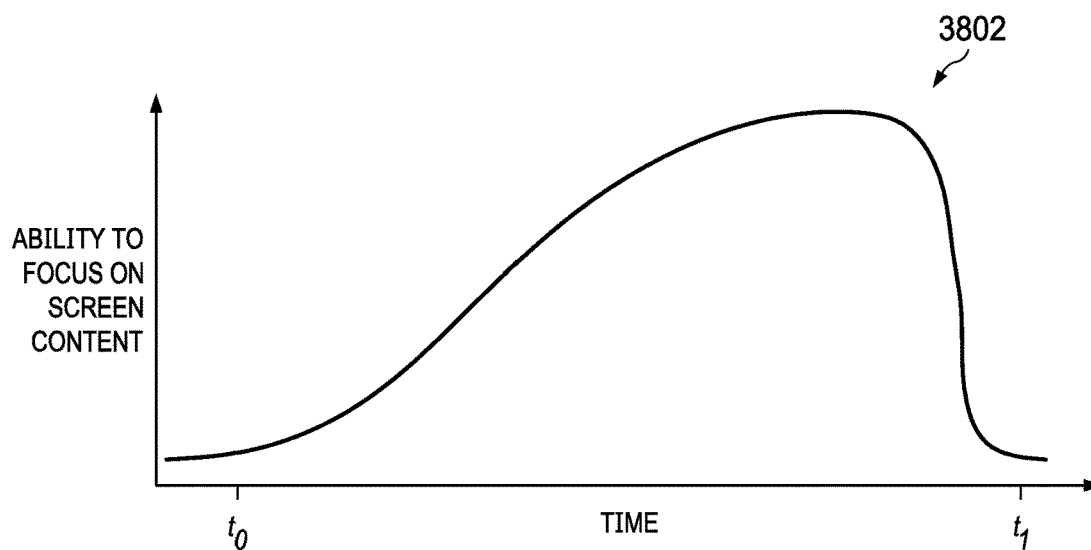


FIG. 38

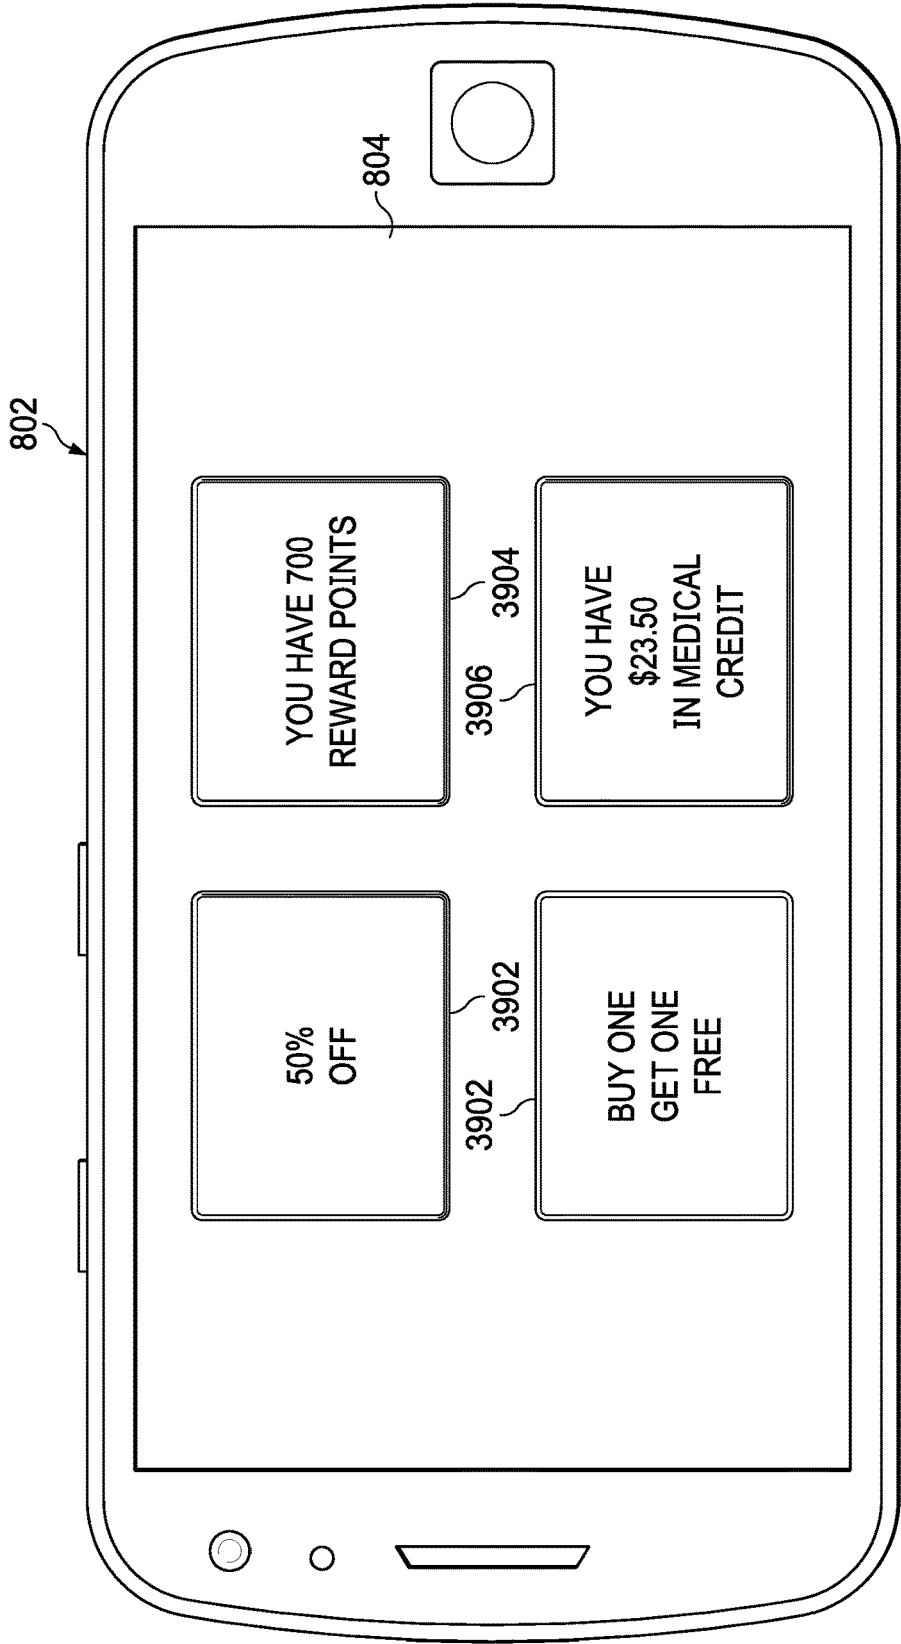


FIG. 39

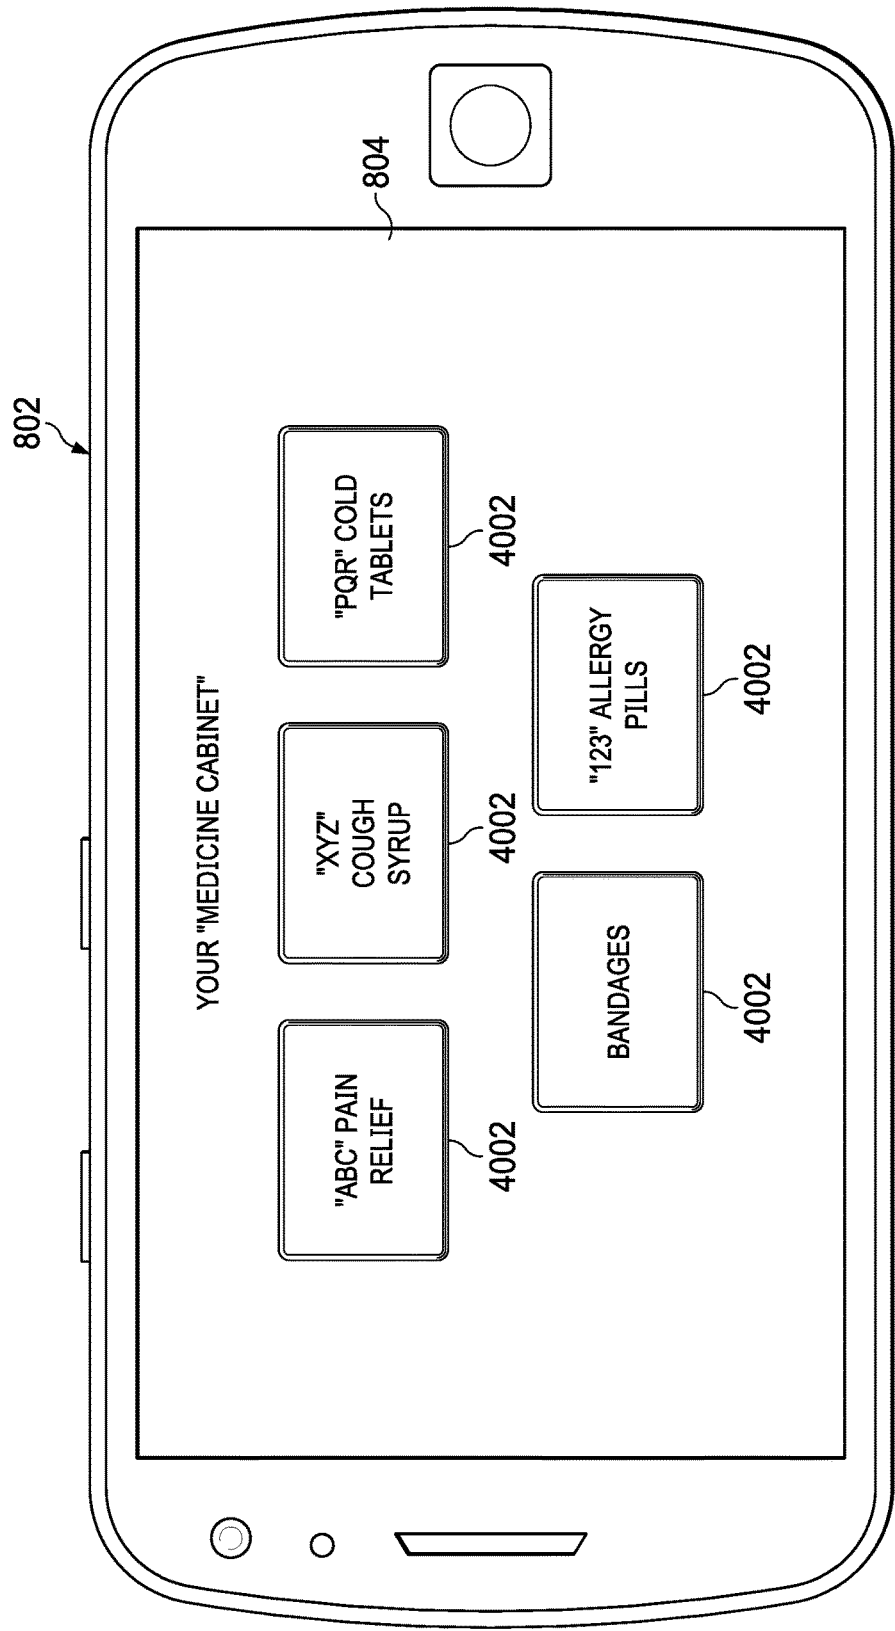


FIG. 40

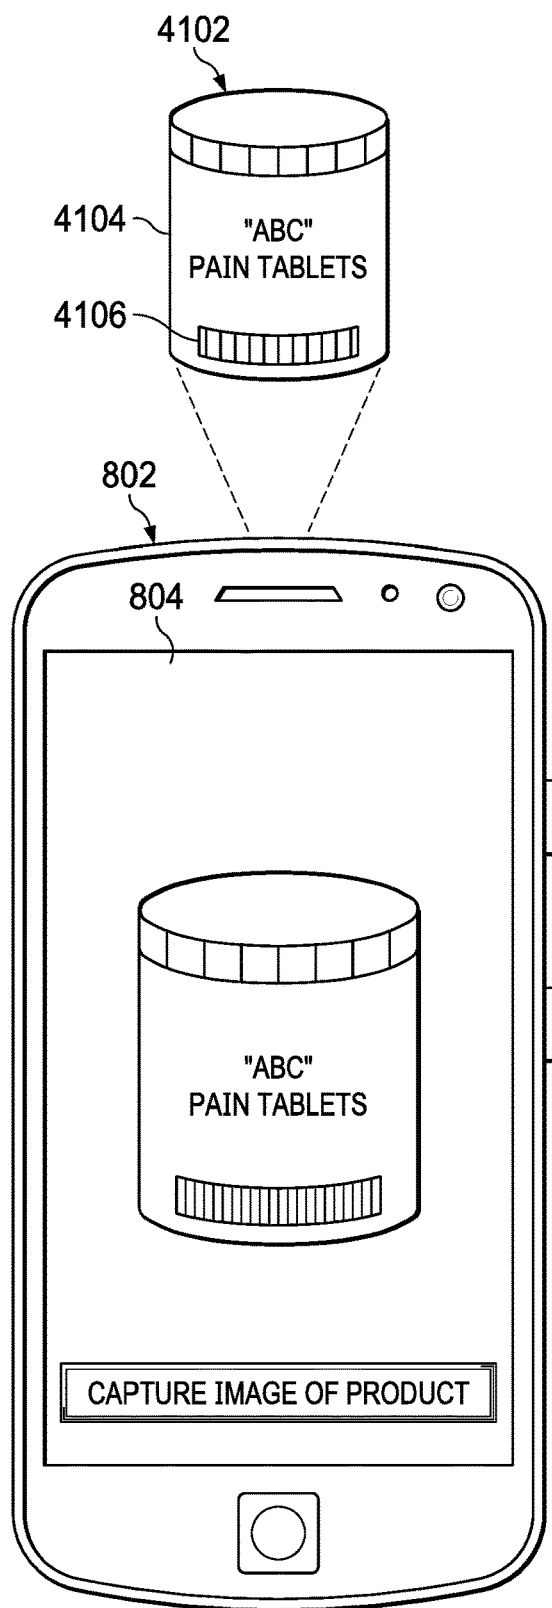


FIG. 41

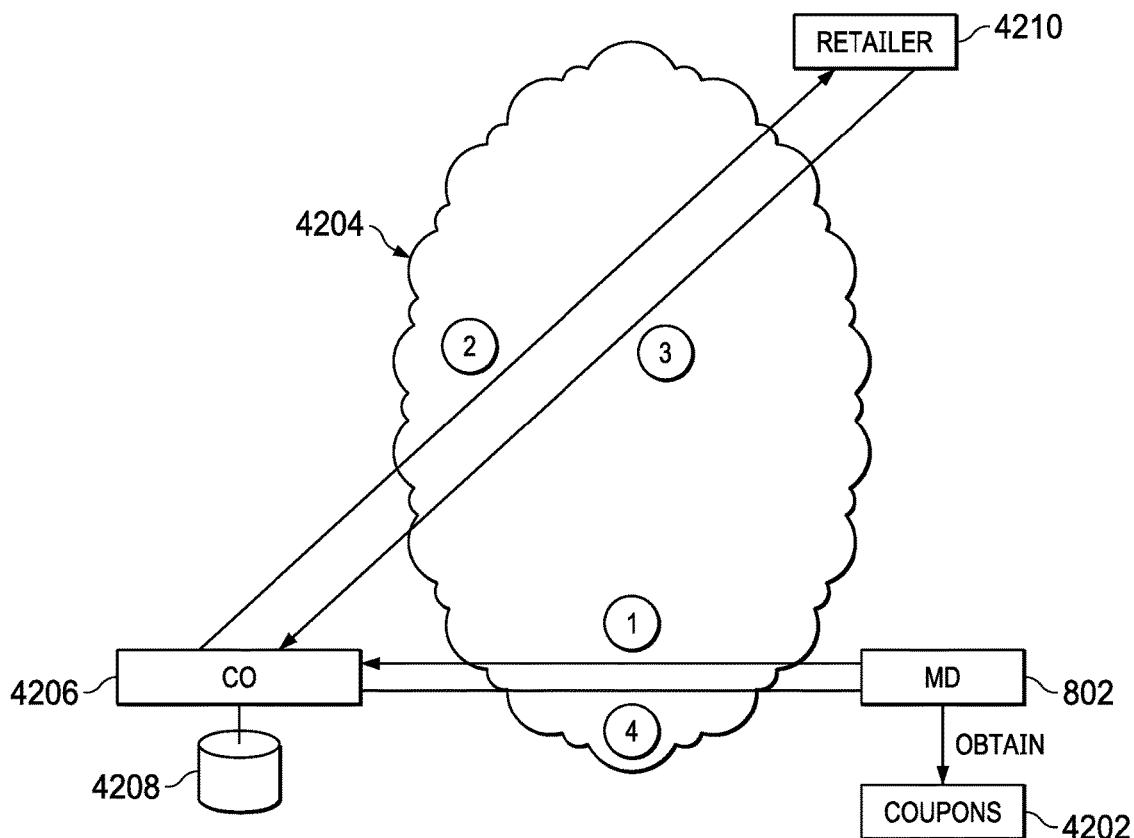


FIG. 42

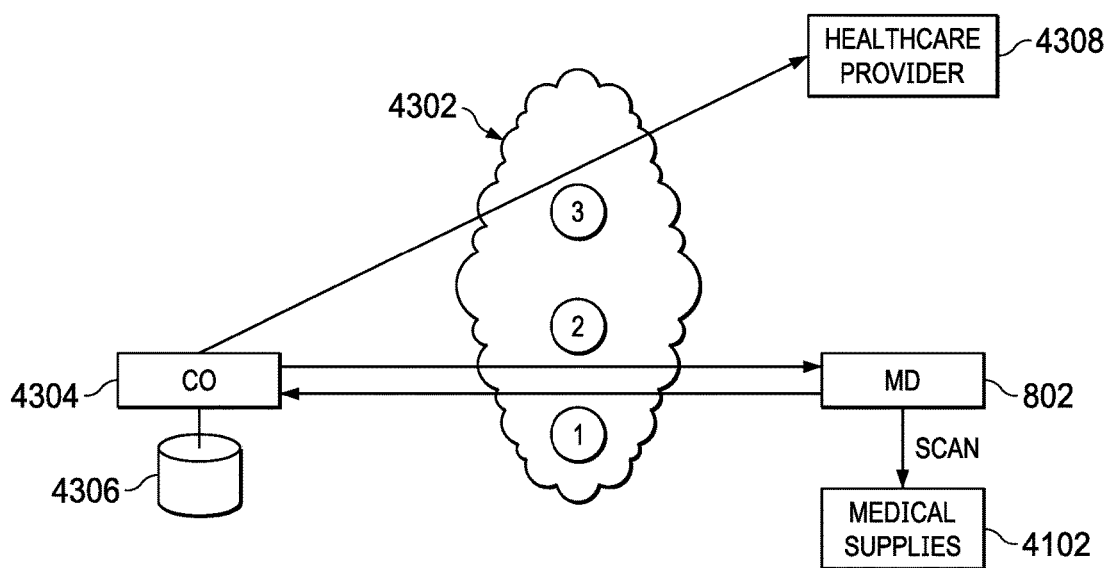


FIG. 43

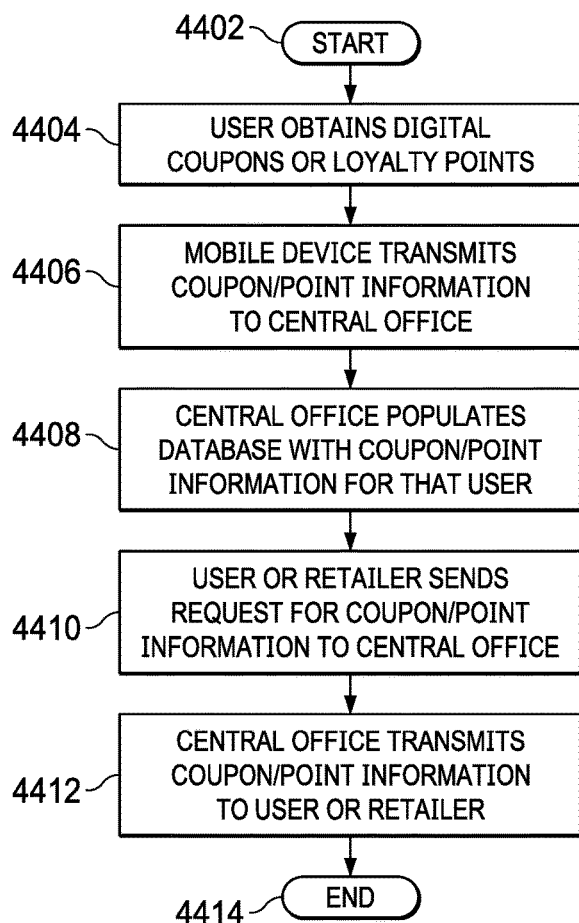


FIG. 44

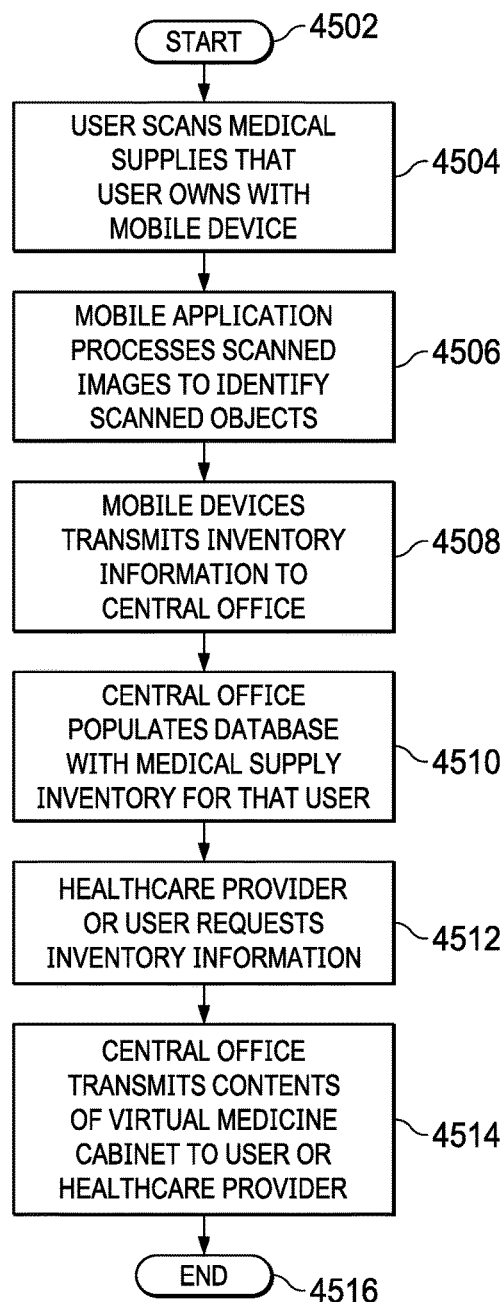


FIG. 45

## SYSTEM AND METHOD FOR A DIGITAL CONSUMER MEDICAL WALLET AND STOREHOUSE

### CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation-in-part of U.S. patent application Ser. No. 15/804,990, filed on Nov. 6, 2017, which is a continuation-in-part of U.S. patent application Ser. No. 15/295,398, filed on Oct. 17, 2016, which issued as U.S. Pat. No. 9,857,373 on Jan. 2, 2018. U.S. patent application Ser. No. 15/804,990 also claims the benefit of U.S. Provisional Application No. 62/419,382, filed on Nov. 8, 2016. This application also claims the benefit of U.S. Provisional Application No. 62/566,598, filed on Oct. 2, 2017. The contents of application Ser. Nos. 15/804,990, 62/419,382, and 62/566,598, and the contents of U.S. Pat. No. 9,857,373, are incorporated by reference herein in their entireties.

### TECHNICAL FIELD

[0002] The following disclosure is related to self-diagnostic tests and, more specifically, delivering advertising to users in response to test results.

### BACKGROUND

[0003] When a user conducts a self-diagnostic test, the user's future buying habits may be influenced by the results of the test. Therefore, it is desirable to have a system and method for delivering advertisements to a user which reflect the results of the test.

### SUMMARY

[0004] In one aspect thereof, a system and method are provided for collection and testing of a biologic sample. The system and method comprise collecting by a user of a testing device a biologic sample for use with the testing device, assigning correlative values as test results, and receiving the test results at a server disposed on a network. Some aspects further include presenting advertisements and other messages to users through a mobile application operating on a mobile device. These aspects take into account the results of the self-diagnostic test and present different advertisements to the user based on the results of the test.

### BRIEF DESCRIPTION OF THE DRAWINGS

[0005] For a more complete understanding, reference is now made to the following description taken in conjunction with the accompanying Drawings in which:

[0006] FIG. 1 illustrates a diagrammatic representation of one embodiment of an immunoassay test strip;

[0007] FIG. 2 illustrates a diagrammatic representation of one embodiment of an immunoassay test wherein an analyte is tested across a plurality of test strips;

[0008] FIG. 3 illustrates a diagrammatic representation of one embodiment of a testing device;

[0009] FIG. 4 illustrates a top view of the testing device of FIG. 3;

[0010] FIG. 5 illustrates a top view of one embodiment of a testing device;

[0011] FIG. 6 illustrates a top view of another embodiment of a testing device;

[0012] FIG. 7 illustrates a flowchart of one embodiment of a testing device use method;

[0013] FIG. 8A illustrates a diagrammatic representation of one embodiment of a process for a mobile device application for testing device image capture and image processing, wherein an image alignment indicator is not aligned with the subject of the image;

[0014] FIG. 8B illustrates a diagrammatic representation of one embodiment of a process for a mobile device application for testing device image capture and image processing, wherein an image alignment indicator is aligned with the subject of the image;

[0015] FIG. 9 illustrates a flowchart of one embodiment of an image analysis process using a mobile device;

[0016] FIG. 10 illustrates a diagrammatic representation of another embodiment of a process for a mobile device application for testing device image capture and image processing, wherein an image alignment indicator is aligned with the subject of the image;

[0017] FIG. 11 illustrates one embodiment of a consumer driven biologic and disease data collection system;

[0018] FIG. 12 illustrates one embodiment of a consumer driven biologic and disease data collection system;

[0019] FIG. 13 illustrates an example of a unique biologic ID database table;

[0020] FIG. 14 illustrates a flowchart of one embodiment of a biologic data collection and dissemination process;

[0021] FIG. 15 illustrates a perspective view of a system for scanning test strips;

[0022] FIG. 16 illustrates a cross-sectional view of the system of FIG. 15;

[0023] FIG. 17 illustrates one embodiment of a vertical flow immunoassay device;

[0024] FIG. 18 illustrates a cross-sectional view of one embodiment of the vertical immunoassay device of FIG. 17;

[0025] FIG. 19 illustrates a color gradient chart;

[0026] FIG. 20 illustrates a normalized past tests results rating chart;

[0027] FIG. 21 illustrates a mobile device displaying on a screen a mobile application variable test functionality;

[0028] FIG. 22 illustrates the mobile device of FIG. 21, wherein a housing of a testing device also includes thereon test function indicators;

[0029] FIG. 23 illustrates a mobile device displaying audiovisual instructions for performing a self-diagnostic test;

[0030] FIG. 24 illustrates a process for using a mobile device camera to capture an image of a scan-able code to determine which set of instructions is correct for a self-diagnostic test;

[0031] FIG. 25 illustrates a process for entering a product code into a mobile device on a mobile application for the purpose of obtaining instructions for a self-diagnostic test;

[0032] FIG. 26 illustrates an acknowledgement screen on a mobile application for a user to acknowledge understanding self-diagnostic test instructions;

[0033] FIG. 27 illustrates a flowchart depicting a process for presenting self-diagnostic test instructions to a user;

[0034] FIG. 28 illustrates a flowchart for generating test results with a remote server and database from an image communicated by a mobile application on a mobile device;

[0035] FIG. 29 illustrates a mobile device displaying audiovisual messages to a self-diagnostic test user;



[0036] FIG. 30 illustrates a flowchart depicting a process for presenting audiovisual messages to a self-diagnostic test user;

[0037] FIG. 31 illustrates a mobile device presenting a variety of types of advertisements to a self-diagnostic test user;

[0038] FIG. 32 illustrates a flowchart depicting a process for presenting advertisements to a self-diagnostic test user;

[0039] FIG. 33 illustrates a mobile device presenting audiovisual messages and advertisements to a self-diagnostic test user;

[0040] FIG. 34 illustrates a mobile device presenting advertisements based on self-diagnostic test results to a self-diagnostic test user;

[0041] FIG. 35 illustrates a flowchart depicting the process for presenting advertisements based on self-diagnostic test results to a self-diagnostic test user;

[0042] FIG. 36 illustrates a system for delivering content to a mobile application;

[0043] FIG. 37 illustrates several relational databases for correlating content;

[0044] FIG. 38 illustrates a graph depicting the ability of self-diagnostic test users to focus on a mobile device screen;

[0045] FIG. 39 illustrates an embodiment which includes a digital medical wallet and storehouse;

[0046] FIG. 40 illustrates an embodiment in which the mobile application stores a record of the medical supplies the user already owns;

[0047] FIG. 41 illustrates an embodiment which allows a user to add medication to a "virtual medicine cabinet" by photographing the medication to be added;

[0048] FIG. 42 illustrates an embodiment of a system which includes a digital consumer wallet;

[0049] FIG. 43 illustrates an embodiment of a system which provides a virtual medicine cabinet;

[0050] FIG. 44 illustrates a flowchart for an embodiment which includes a digital consumer wallet; and

[0051] FIG. 45 illustrates a flowchart for an embodiment which includes a virtual medicine cabinet.

#### DETAILED DESCRIPTION

[0052] Referring now to the drawings, wherein like reference numbers are used herein to designate like elements throughout, the various views and embodiments of an arbovirus indicative birth defect risk test are illustrated and described, and other possible embodiments are described. The figures are not necessarily drawn to scale, and in some instances the drawings have been exaggerated and/or simplified in places for illustrative purposes only. One of ordinary skill in the art will appreciate the many possible applications and variations based on the following examples of possible embodiments.

[0053] Referring now to FIG. 1, there is illustrated one embodiment of an immunoassay test strip 100. The test strip 100 is typically housed in a testing device configured to collect a biologic analyte 106 from a user and to direct to the biologic analyte 106 onto the testing strip 100. However, it will be understood that the biologic may be applied onto a strip 100 without the strip 100 needing to be within a testing device. The test strip 100 includes a backing 102. The test strip 100 is made up of multiple sections disposed on the backing 102. A sample pad 104 is disposed on one end of the strip 100, for collecting the biologic analyte 106. The biologic analyte 106 may be any biologic needed for use in

the immunoassay, such as urine, blood, saliva, stool, sweat, or other biologics to be used as an analyte. Various methods may be used to acquire the needed biologic, and such may be provided to the user packaged with the test, such as swabs, vials, containers, dilutants and other solutions, or any other equipment required. In the case of a blood analyte, a few drops of blood may be obtained from a finger stick using a finger prick device. Such a blood analyte may be blood mixed with an adequate amount of buffered solution to create the sample analyte 106 or a blood sample that is not diluted or otherwise manipulated, in which case the blood only is the analyte 106.

[0054] The biologic analyte 106, after coming into contact with the sample pad 104, begins to migrate across the strip 100 by capillary action, coming into contact with other sections of the strip 100. A particle conjugate pad 108 is disposed between the sample pad 104 and a test line 110. The conjugate pad 108 may contain various reagents associated with a particular antigen, such as a virus, allergen, or bacteria, the reagents being items such as antibodies, enzymes, or other reagents needed to diagnose the particular condition. The reagent in the conjugate pad 108 may be conjugated with particles of materials such as colloid gold or colored latex beads. As the analyte 106 migrates through the conjugate pad 108, antibodies present in the sample analyte 106 complex with the reagents in the conjugate pad 108, thereby creating an immune complex that will migrate to the test zone or test line 110.

[0055] The test line 110 (T) may be precoated with the relevant antigen in question, i.e., a virus, allergen, or bacteria, for the detection of antibodies associated with the particular antigen. The immune complex created when the analyte 106 passes through the conjugate pad 108 is captured onto the antigen contained on the test line 110. This may create a qualitative response on the strip where the test line 110 is located, such as a colored response. In some embodiments, the test line 110 may not be a line, but may be other shapes or symbols, such as a plus sign. If no antigen-anti-antigen complexes are present in the analyte, no reaction occurs in the test line 110 and a qualitative response will not occur.

[0056] After passing through the test line 110, the analyte migrates further along the strip to reach a control line 112, where excess anti-antibody-colloidal gold or latex conjugates get bound. A qualitative response may be shown at the control line 112, indicating that the sample has adequately migrated across the testing membrane or substrate as intended. It will be understood that the control line 112 is not necessarily needed to perform the test, and may be eliminated entirely, but the control line 112 does provide a comparative example for a user reading the test. For example, the control line 112, in embodiments where a colored qualitative response is provided, may appear as an overly saturated color, such as a dark or bright saturated red, once the sample reaches the control line 112. This saturated color may be used as a comparison against the qualitative response shown on the test line 110. For example, if the qualitative response shown on the test line 110 is a much lighter red than that on the test line 110, it may be that very little reaction occurred at the test line. Of course, if no response is shown at all at the test line 110, no reaction has occurred. If the qualitative response at the test line 110 is of a similar saturation to the control line 112, a strong reaction is indicated.

[0057] The strip 100 may not be a continuous substrate. Rather, the various sections of the strip 100 may be separate from each other, but all adhered to the backing 102. As shown in FIG. 1, the sample pad 104 and the conjugate pad 108 are separate structures from each other. The test line 110 or zone and the control line 112 or zone are both disposed as part of a nitrocellulose membrane strip 114. The nitrocellulose membrane strip 114 is also adhered to the backing 102, but separate from the sample pad 104 and the conjugate pad 108. As shown in FIG. 1, the end of the sample pad 104 adjacent to the conjugate pad 108 may overlap the conjugate pad 108, with that end of the sample pad 104 lying over the adjacent end of the conjugate pad 108. Similarly, the end of the conjugate pad adjacent to the nitrocellulose membrane strip 114 may lie over the end of the nitrocellulose membrane adjacent to the conjugate pad. This allows for the analyte 106 to be more easily deposited onto each section of the strip 100 as it migrates across the strip 100. After the analyte 106 migrates across the nitrocellulose membrane strip 114, and thus across the test line 110 and the control line 112, the analyte 106 comes into contact with a wick 116 for absorption and collection of the analyte 106. The end of the wick 116 adjacent to the nitrocellulose membrane strip 114 may lie over that adjacent end of the nitrocellulose membrane strip 114, as shown in FIG. 1.

[0058] Several Flow Immune Assays have been directed toward identifying proteins, molecules of interest, and even immunoglobulins IgG, IgA, and IgM. IgE is an antibody (immunoglobulin E) that is normally present in the blood freely circulating until it moves into the tissue where it is bound to mast cells through the receptor Fc $\epsilon$ RI (F-C-epsilon-R-one) otherwise known as the high affinity IgE receptor. There is a small amount of IgE bound to IgE receptors (high and low affinity receptors) on basophils, eosinophils, and other cells in the blood and tissues.

[0059] Many assay systems are geared toward the detection of infectious proteins. All of the aforementioned tests use a non-human antibody—usually IgG type—e.g., goat IgG antibody directed against a protein of interest to detect the protein of interest from the sample (blood, urine, saliva, sweat, etc.). This antibody complexes with protein of interest and forms a complex that travels across the membrane until it reaches the test zone. In the test zone there is an IgG type antibody directed against IgG from that species of animal. As further described herein, the present detecting apparatus and method use human (patient/consumer-derived) antibodies from the sample and the test zone that contains a humanized antibody directed against the protein of interest that is pre-conjugated to a detecting substance that results in a visual change.

[0060] Summary of Target Antigen:

[0061] The target antigens may be proteins, glycoproteins, lipoproteins or other molecular substances capable of eliciting an immune reaction and/or being bound by human specific IgE (sIgE).

[0062] Immune Assay to Detect Specific IgE:

[0063] In the detecting apparatus and method of using the same, the antigens are proteins conjugated to a noble metal, for example, gold, or latex conjugated to antigen in the test zone, for the purpose of detecting the presence of specific IgE (e.g., anti-peanut IgE in a blood sample from a finger prick). For example, an IgG class antibody (IgG1, IgG2, IgG3, or IgG4) or fragments of those classes of antibodies (fab fragments) whose origin may be any animal species

(goat, rat, human, etc.) capable of detecting human IgE (anti-IgE IgG)—a suitable commercially available humanized antibody, such as omalizumab may be used—may be used to form immune complexes of IgG-anti-IgE-sIgE that will migrate to the test zone having selected specific IgE that can bind to the conjugated antigen.

[0064] Immune Assay to Detect Total IgE (not Concerned about Specific IgE):

[0065] Another embodiment includes using an IgG class antibody (IgG1, IgG2, IgG3, or IgG4) or fragments of those classes of antibodies (fab fragments) whose origin may be any animal species (goat, rat, human, etc.) capable of detecting human IgE (anti-IgE IgG)—a suitable commercially available humanized antibody that is pre-conjugated to a detecting molecule that results in a color change when bound to IgE as the target antigen in the test zone.

[0066] Referring now to FIG. 2, there is illustrated one embodiment of an immunoassay test 200 wherein an analyte 202 is tested across a plurality of test strips 204. The plurality of test strips 204 may each be configured for testing for a particular antigen. For instance, one strip may be for testing for the presence of streptococcal bacteria (strep throat), one strip may be for testing for a peanut allergy, one strip may be for testing for the Zika virus, etc. Additionally, each strip may also test for multiple antigens. For example, as shown in FIG. 2, multiple testing panels or lines may be incorporated. Each line may be for a particular antigen. As shown in FIG. 2, multiple test lines 206, 208, and 208 may be disposed along the plurality of strips 204. A strip testing for allergens may have a panel for testing for peanut allergies shown at test line 206 (CH1), for cat allergies shown at test line 208 (CH2), or grass allergies shown at test line 210 (CH3).

[0067] Other examples of configurations for the testing panels can be, but are not limited to: 1) Food 5: Peanut, milk, soy, wheat, egg; 2) Nut and seed panel: almond, cashew, hazelnut, peanut, pecan, walnut, sesame seed, sunflower seed; 3) seafood: crab, lobster, shrimp, salmon, tuna; 4) Pets: cat, dog; 5) Indoor allergens: dust mites, mold mix (*alternaria*, *aspergillus*, *penicillium*, *cladosporium*), cat, dog; and 6) seasonal allergens: grass (Bermuda, bahia, Johnson, rye, timothy), trees (oak, elm, cedar, mesquite, pine, etc.), weeds (pigweed, ragweed, sage, Russian thistle).

[0068] With respect to other non-allergen antigens, the panels may be for testing for strep, Zika, flu, anthrax, cold viruses, cancer, HPV, Lyme disease, mononucleosis (mono), and other illnesses, and/or other conditions such as pregnancy (hCG detection) and disease risks. Some embodiments may allow for the testing of various arboviruses (arthropod-borne viruses). Arboviruses are viruses that are transmitted by arthropods, with mosquitoes being a common vector for the virus. Vectors are organisms that transfer the virus from a host that carries the virus. Thus, in the case of mosquitoes, a mosquito that feeds on a host that is infected with a virus may infect others when that mosquito again feeds on an uninfected host. Well-known arboviruses include Dengue virus, Japanese encephalitis virus, Rift Valley fever virus, West Nile virus, yellow fever virus, chikungunya, and Zika virus. Urine, blood, and saliva and other biologics may be used for arboviruses testing.

[0069] Certain antigens or medical conditions may be logically paired together. For instance, a testing device may include both a strip for detection of pregnancy and a strip for the detection of the Zika virus, as the Zika virus has been

known to cause birth defects in infants born to pregnant women that are infected with Zika. Thus, combining these two tests into a single testing device or kit would alert a woman to a potential Zika infection proximate in time to the time she also discovers she is pregnant, allowing the woman to seek medical attention immediately. This is a substantial improvement over past Zika testing, where a woman may be required to wait weeks before results are returned from a lab after having the biologic collected by her physician. In many cases, this may lead to a woman having passed a state-mandated cutoff point for abortions, such as 24 weeks in some states. Combining a Zika test with a pregnancy test and physically linking the two tests, and thus allowing for a woman to determine a Zika risk at the time of taking a pregnancy test, in which a pregnancy test may be taken as soon as six days after conception, allows for that woman to take action much sooner than the state mandated cutoff and waiting for lab results would allow.

**[0070]** Various testing devices that include the test strip **100** or strips may be used, such as a slide that supports the test strip **100**, a cassette based diagnostic test, a dipstick, or combinations thereof. The test results in various embodiments may be in the form of a visual qualitative reading test, a visual semiquantitative format, a reader quantitative assay format, and/or combinations thereof. Additionally, an electronic implementation may be used where the result is displayed digitally on a screen disposed within the apparatus, and visible to the user.

**[0071]** The apparatus and method of detection may be a “one-step” approach from sample to reading without sample dilution or other sample manipulation. The sample may be diluted or endure other sample manipulation, for example the blood sample is diluted with a buffer.

**[0072]** Referring now to FIG. 3, there is illustrated a diagrammatic representation of one embodiment of a testing device **300**. The testing device **300** includes a housing **302** that forms the body of the testing device. The housing **302** may be made of plastic, metal, or any material durable enough for shipping and subsequent handling by a user. The housing **302** may be hollow so that a plurality of test strips **304** may be housed within and so that a biologic may be deposited within the housing **302**. The testing device **300** may further have a plurality of windows **306**, each window being associated with one of the plurality of test strips **304**, and allowing for a user to view at least the section of the nitrocellulose membrane strip **114** where the test line **110** and control line **112** are located. The plurality of windows **306** may be open, or covered with plastic, glass, or other materials that allow for viewing the plurality of strips **304**. A sample well **308** may be disposed on a surface of the housing **302** to allow a user to deposit a biologic into the housing **302**. The sample well **308** would be disposed over or near the sample pad **104** of the test strip or strips **100**. In the embodiment shown in FIG. 3, a single sample well **308** is included for collection of a single type of biologic for testing, with each of the plurality of strips **304** being suited for testing for antigens using that particular biologic sample type. For example, if the testing device **300** is a combined pregnancy and Zika test, having both a pregnancy strip and a Zika strip, a urine sample may be deposited into the sample well **308**, causing the urine sample to come into contact with the sample pad **104** on both the pregnancy strip and the Zika strip. It will be understood that both of these tests may also be performed with a blood sample.

**[0073]** The testing device **300** may also have disposed on the surface of the housing a crosshair symbol **310**, used as an alignment target. This symbol may be a graphic printed or adhered to the testing device **300**. The crosshair symbol **310** is used to align the testing device **300** for the taking of an image of the testing device **300** using a camera on a mobile device, for use in a mobile device application described herein. In other embodiments, the crosshair symbol **310** may be other types of symbols, such as a simple shape (circle, square, etc.), other images (such as a medical cross symbol, an arrow, etc.), or any other type of image.

**[0074]** Referring now to FIG. 4, there is illustrated a top view of the testing device **300**. There is again shown the housing **302**, the plurality of test strips **304**, the plurality of windows **306**, the sample well **308**, and the crosshair symbol **310**.

**[0075]** Referring now to FIG. 5, there is illustrated a top view of one embodiment of a testing device **500**. The testing device **500** includes a housing **502** having a plurality of test strips **504** within the housing **502** and a plurality of windows **506** for display of the plurality of strips **504**. The housing **502** also includes a plurality of sample wells **508** disposed on one side of the testing device **500**. Each of the plurality of sample wells **508** is associated with one of the plurality of test strips **504** and each of the plurality of sample wells **508** may be disposed over one of the sample pads **104** on the associated one of the plurality of test strips **504**. This allows for a biologic to be deposited into each of the plurality of sample wells **508**, with each well **508** serving to transfer the biologic to the test strip underneath the sample well. The testing device **500** further includes a crosshair **510**. The crosshair symbol **510** is used to align the testing device **500** for the taking of an image of the testing device **500** using a camera on a mobile device, for use in a mobile device application described herein.

**[0076]** Referring now to FIG. 6, there is illustrated a top view of another embodiment of a testing device **600**. The testing device **600** includes a housing **602** having a plurality of test strips **604** within the housing **602** and a plurality of windows **606** for display of the plurality of strips **604**. The housing **602** also includes a plurality of sample wells **608**. In this embodiment, the sample wells are located on different ends of the housing **602**. In the case of a two test strip device, the sample wells **608** are disposed on opposite ends of the testing device **600**. The strips **604** would be arranged within the housing in such a way as to allow the sample pad **104** on each of the strip to be disposed underneath one of the sample wells **608**. This is useful for testing devices that require different biological samples. For example, if the testing device **600** required a urine sample for one strip and a blood sample for the other strip, having the wells **608** disposed on opposite sides of the testing device would reduce the likelihood that a urine sample, for instance, might be inadvertently deposited into the well designated for the blood sample. In embodiments where there are more than two strips, and more than two wells, the well positions may alternate between the two sides of the testing device. For instance, a first well for a first strip might be disposed on the left side of the testing device, a second well for a second strip might be disposed on the right side of the testing device, a third well for a third strip might be disposed on the left side of the testing device, a fourth well for a fourth strip might be disposed on the right side of the testing device, and so on. The testing device **600** further includes a crosshair

**610.** The crosshair symbol **610** is used to align the testing device **600** for the taking of an image of the testing device **600** using a camera on a mobile device, for use in a mobile device application described herein.

**[0077]** The diagnostic test can, for example, be produced in a various formats for different users, such as, but not limited to, consumer/in-home use where the test is purchased through retail channels which will allow individuals to get an immediate, cost-effective test result that can lead to specific avoidance and treatment through follow-up with a medical professional.

**[0078]** The diagnostic test can be provided to and used by hospitals and clinics to provide rapid, on-site test results that are required to prescribe certain medications, such as omalizumab, by their FDA labels.

**[0079]** This diagnostic assay can be modified to detect the presence of specific IgE in pets.

**[0080]** It is also noted that housing **602** is designed such that both strips **604** are disposed in physical proximity thereto and in the same actual housing. In this manner, both sets are linked physically to each other such that they cannot be separated and can be associated with a single individual and the actual test cannot be separated. As such, when a patient applies the specimens to the two areas **608** and the test results are exhibited, there is a high probability that two tests were performed at the same time associated with the same patient. Additionally, and electronic chip (not shown) can be embedded within the housing **602** such that the housing **602** can be registered to a specific patient and associated with the medical records of that patient.

**[0081]** Referring now to FIG. 7, there is illustrated a flowchart of one embodiment of a testing device use method **700**. The method **700** begins at step **702** where a biologic is collected in a sample well or wells of a testing device. The biologic collected may be a non-diluted or non-manipulated biologic, such as blood, urine, or saliva from the user of the test. Diluted or manipulated biologics may be used instead, as required by the specific test. For example, if a viral test requires the biologic to be added to a solution, the biologic could be added to a solution that has previously been placed in a sterilized vial provided with the testing device. After the required amount of time has passed, the solution containing the biologic could be deposited into the well or wells. At step **704**, the biologic contacts a sample pad disposed on a strip or strips within the testing device. At step **706**, the biologic migrates along the strip or strips to come into contact with a conjugate pad containing antibodies. Antibodies present in the biologic will complex with the antibodies in the conjugate pad to create an immune complex. At step **708**, the biologic migrates into a test zone of the strip or strips, coming into contact with an antigen. The antibodies in the conjugate pad serve to provide a means of detection, such as a colored response, if the immune complex binds with the antigen present in the test zone of the strip. At decision block **710**, binding of the antibodies with the antigen may or may not occur depending on if antibodies associated with the antigen are present in the biologic or not. If a binding between the antibodies and the antigen does not occur the process moves to step **712** where no qualitative response is produced on the test line. If a binding does occur, at step **714** a qualitative response is produced on the test line. Whether a binding occurs or not, and whether a qualitative response is produced or not, the process moves to step **716** where the biologic migrates into a control zone of the strip or strips

where excess conjugates get bound and produces a qualitative control zone reaction indicating that the sample has adequately migrated across the testing zone.

**[0082]** It will be understood by one skilled in the art that the antibodies and antigens applied to the testing strip may be altered depending on the type of condition being tested. For example, in the case of testing for medical conditions that do not involve an illness or infection, like pregnancy, and thus the sample biologic does not contain antibodies associated with the condition, antibodies that react to markers being tested for may be applied to the testing strip instead of an antigen. For instance, pregnancy test requires testing for the presence of hCG. Since hCG is a hormone and not an antibody produced in response to an infection, the testing strip may have antibodies that will react to the presence of hCG applied to the testing zone or line of the testing strip, as well as to the conjugate pad. Similarly, some tests might require antibodies be applied to the testing strip to detect antigens present in the sample, rather than antibodies.

**[0083]** Referring now to FIGS. 8A and 8B, there is illustrated a diagrammatic view of one embodiment of a process **800** for a mobile device application for testing device image capture and image processing. The mobile device application allows for an image of a testing device, such as testing device **300**, to be captured using a camera installed on a mobile device **802** having a screen **804**. While the mobile device **802** displays on the screen **804** the scene captured by the camera, the mobile device application also displays a graphic on the screen **804** in the form of a boxed outline **806**, the size of the outline **806** corresponding to the size of the testing device **300**. Also displayed on the screen of the mobile device **802** within or near the outline is a crosshair graphic **808**. A user of the mobile device **802** attempts to align the outline **806** with the borders of the testing device **300** and also attempts to align the crosshair graphic **808** with the crosshair **310** on the testing device **300**. While alignment has not yet been achieved, a misalignment warning **810** may appear on the screen of the mobile device **802**, indicating to the user that alignment has not yet been achieved. Such is shown in FIG. 8A.

**[0084]** In FIG. 8B, there is shown the result of a successful alignment of the outline **806** with the testing device **300** and successful alignment of the crosshair graphic **808** with the crosshair **310** on the testing device **300**. As shown in FIG. 8B, once aligned, a success indicator **812** may appear, such as a check mark or other positive status symbol, on the aligned image. Successful alignment causes the camera on the mobile device **802** to capture the current image of the testing device **300**. Other checks may occur, including ensuring that the image is focused before the image is saved. This image is then processed to determine a result based on the severity of the reaction occurring on the test strip. The mobile device application performs an analysis of the test line captured in the image, counting the number of colored pixels, as well as determining the intensity of the color. The mobile device may then compare this number and color intensity to that in the control line, providing a mathematical evaluation of the test line. Utilizing unique wavelengths of light for illumination in conjunction with either CMOS or CCD detection technology, a signal rich image is produced of the test lines to detect the colloid gold or latex particles. This provides an advantage because a user simply looking at the two lines may not know what the test line indicates, such as when the colored line does appears on the strip, but it is

a faded line, rather than a dark line. Based on this analysis, the mobile device application may provide a results indicator **814**.

**[0085]** The results indicator **814** may be a qualitative result or a quantitative result. For example, and as shown in FIG. **8B**, a qualitative result for the results indicator **814** may indicate, in the case of a testing device for testing pregnancy as well as an infection, a plus sign next to a line reading “pregnant:” and a plus sign next to a line reading “infection:” to indicate that the user is both pregnant and infected with the bacteria or virus being tested, such as the Zika virus. For a quantitative result, the results might provide a numeric rating. For instance, a rating system between 1-100 may be used. If the results provide a low rating to the user, such as a rating of **10**, this indicates a low risk of infection, although medical attention may be sought by the user anyway. For example, if the user is pregnant, and also receives a **10** rating for Zika, this may indicate that Zika was detected in low amounts. However, the user may still seek medical attention or further testing from her doctor because Zika has been known to cause birth defects. If the rating is a high rating, such as **95**, this indicates that an infection has most likely occurred and medical attention should be sought immediately.

**[0086]** This same quantitative rating system may be applied to any test (viral infections, bacterial infections, pregnancy, and other health conditions), as the quantitative test can be performed using the software described herein to accurately test bound antibody concentrations on the test strip. In some embodiments, a combined qualitative and quantitative result may be presented, such as both a rating and a plus or minus sign being presented, or other types of quantitative and qualitative indications. Additionally, various combinations of tests may be provided for in the testing device, such as pregnancy/Zika, pregnancy/flu, pregnancy/strep/Zika, etc.

**[0087]** Referring now to FIG. **9**, there is illustrated a flowchart of one embodiment of an image analysis process **900** using a mobile device. At step **902** a mobile device application is launched. At step **904** a camera on the mobile device is activated and a crosshair indicator and a testing device outline appear on the mobile device screen. At step **906** the crosshair indicator presented on the screen of the mobile device is aligned with a crosshair icon on the testing device and the device outline presented on the screen of the mobile device is aligned with the borders of a testing device. At step **908**, an indicator of successful alignment is presented on the screen and an image of the testing device is taken by the mobile device camera. At step **910**, the mobile device application processes the image of the testing device to determine test line strength by counting the number of colored pixels contained in the test line. At step **912**, the mobile device application correlates line intensity with analyte concentrations to further determine test line strength. At step **914**, the mobile device application presents the test results based on pixel count and line intensity, providing either a qualitative or quantitative result.

**[0088]** In some embodiments, the number of pixels indicating bound antibodies on the strip may be measured against that in the control line to compare line intensity between the two lines, with the control line acting as an example of a strong reaction, indicating a strong infection, and determining how close the test line intensity is to the control line. This would lead to a logical quantitative result.

For instance, if the test line is determined to have a pixel count and line intensity that is 25% of the pixel count and line intensity of the control line, a rating of **25** may be given. If a qualitative result is to be provided, a rating of **25** may give a qualitative result that is negative, or it could be positive depending on the type of condition being tested and known actual infection results where a rating of **25** occurred for that condition.

**[0089]** In some embodiments, the test line may not be compared with the control line to determine a result. Rather, the mobile device application may have access to a database having data on numerous past tests for the same condition. This data may instead be used as the control. This allows the application on the mobile device to retrieve data on past tests and compare the test line data of the current test to past tests. Overall data for past tests may be provided and compared against, such as providing an average or a curve of past tests, or individual tests rated as having accurate results may be compared against.

**[0090]** In addition to a status result of an infection or other medical condition being provided to the user, other indicators of health may also be tested and results thereon provided. This provides for potential early identification of pregnancy and risk of morbidity, allowing for medical attention to be sought much more quickly. Indicators of health may be detected from biologics, such as urine and blood. Urine, for example, allows for the detection of glucose levels, proteins, bacteria, and infectious markers. In the case of glucose, glucose is usually not found in urine, but, if it is, that is an indicator of extremely high levels of glucose in the body, where the kidneys release excess glucose into urine. This is often a sign of diabetes. Protein in the urine may indicate a malfunctioning of the kidneys, which could be the result of high blood pressure. Similarly, if blood is detected in urine, it could be a sign of a problem with the kidneys or the bladder. Blood, for example, allows for the detection of glucose, inflammation, hormones, genetic defect risks, and metabolic endocrine disorders.

**[0091]** Referring now to FIG. **10**, there is illustrated another embodiment of a successful alignment of the outline **806** with the testing device **300** and successful alignment of the crosshair graphic **808** with the crosshair **310** on the testing device **300**, wherein quantitative results for health risk indicators are provided. In this embodiment, the results indicator **814** provides a qualitative result for pregnancy, and quantitative results for other health risk indicators. In the embodiment shown in FIG. **10**, the health risk indicators being tested are markers for blood pressure and for glucose levels. For blood pressure, this is a test for markers in the blood that can be associated with high blood pressure. These could be test for such things as low levels of vitamin D and the such. Studies have shown that patients suffering from essential hypertension will be under oxidative stress and Malondialdehyde (MDA) is the principal and most studied product of polyunsaturated fatty acid pre-oxidation. This can show an indirect correlation with anti-oxidants, particularly with superoxide dismutases (SODs) ( $r=0.573$ ) and catalase ( $r=0.633$ ) representative anti-oxidant are involved in reducing the stress of a patient's biological system during hypertension. Another marker for hypertension is buildup of uric acid, where in uric acid is a marker for xanthine oxidase-associated oxidants and that the latter could be driving the

hypertensive response. Additional markers are cortisol, a hormone. The test strips **604** can test for the different biological markers.

**[0092]** The results indicator **814** provides numeric ratings, in this case, 1-100, with the blood pressure rating being 88 and the glucose rating being 95. This indicates that both blood pressure and glucose are extremely high. Due to this, an additional alert indicator **1002** is presented to the user on the screen of the mobile device, alerting the user to seek medical attention immediately. This is to ensure that the health of both the pregnant woman and the fetus can be checked as close to the time of pregnancy detection as possible and medical attention received if needed.

**[0093]** Referring now to FIG. **11**, there is provided a flowchart of one embodiment of a pregnancy disease risk assessment process **1100**. The process **1100** begins at step **1102** where a biologic is collected and deposited in a testing device for testing of the biologic. At step **1104**, the biologic is processed by the testing device for detection of pregnancy and various other medical conditions. These medical conditions may be high blood pressure, diabetes, bacterial or viral infections, inflammation, an increase in hormone levels, genetic disease markers, and/or metabolic disorders. At step **1106**, a mobile device is used to capture an image of the testing device after testing is complete. In some embodiments, test results may be immediate. In other embodiments, and depending on the medical conditions being tested, the test may take a certain amount of time to complete. In this case, the user of the test would be alerted to this fact in instructions provided with the testing device. Additionally, a visual indicator on the testing device may alert the user that a test is now complete. At step **1108**, the mobile device provides a rating for each medical condition being tested, such as that described with respect to FIG. **10** herein.

**[0094]** At decision block **1110**, it is determined whether the ratings for each condition exceed a certain threshold for that condition. If not, the process **1100** moves to step **1112**, where an indication is presented to the user via the mobile device screen that medical attention is not currently advised or necessary. If at step **1110** it is determined that at least one of the medical conditions being tested rises above a certain threshold, the process **1100** moves to step **1114** where a warning is presented to the user via the mobile device screen that medical attention is advised. The thresholds for medical conditions may not trigger a warning even if a rating exceeds a threshold, if, in the event of multiple tests being performed, the combined test results do not warrant immediate medical attention. For example, if a user is testing for a cold virus, blood pressure, and glucose, and only the cold virus rating is above the threshold, there may not be a warning provided to the user. Additionally, ratings may be weighted or aggregated based on the medical conditions being tested. For example, if blood pressure, inflammation, and glucose are being tested for, and they all are given only moderate ratings that do not rise above the threshold for any condition individually, an warning to seek medical attention may still be provided due to the combination of conditions taken together.

**[0095]** Referring now to FIG. **12**, there is illustrated one embodiment of a consumer driven biologic and disease data collection system **1200**. Data collected from users performing the tests disclosed herein effectively can provide a wealth of information. As tests are performed data may be passed by a plurality of mobile devices **1202** being used by

users performing tests to a database **1204**, the database being at a remote server **1206**, over a network **1208**. The user is sourcing a biologic from user's own body. This is done at home, not in a lab, hospital, or clinic. Each particular test would expect a certain type of biologic to be provided. For instance, for a pregnancy test, a urine sample is provided and tested for pregnancy markers. For a stool test, the stool might be dissolved in a vial with a solution provided with the testing device/kit, and tested for various disease or infectious markers. Data and results from the tests may be stored on the database **1204** at the remote server **1206**. As described herein, this data may be used as a control for testing analysis for users of the plurality of mobile devices **1202**. This data may also be used to provide data sets for biologics to a medical organization **1210**. The medical organization **1210** may be doctor's offices, researchers, hospitals, testing labs, and other individuals or organizations that have an interest in the health and analysis of users taking the test and of their biologic samples. In this way, data can be gathered from a variety of biologics tested for a variety of different medical conditions and characteristics.

**[0096]** Referring now to FIG. **13**, there is illustrated an example of a unique biologic ID database table **1300**. The table **1300** is illustrative of the type of data stored in association with data for a biologic transmitted by the plurality of mobile devices **1202** for storage on the database **1204**. A biologic ID header **1302** is provided that shows that the biologic sample has been given a unique ID. All data concerning the biologic may be stored in association with the unique biologic ID. The table **1300** also includes a biologic type entry **1306**. This designates what type of biologic that the biologic associated with the unique ID is, such as blood, urine, stool, saliva, sweat, or other biologics. The table **1300** also provides a plurality of test ratings **1304**, for various tests performed on the biologic. In the example shown in FIG. **13**, a blood biologic is provided having an assigned ID of 2402, and having been testing for pregnancy markers, the Zika virus, and for glucose levels. The rating for pregnancy was a 99 rating, the rating for a Zika infection was a 75, and the rating for glucose levels was a 10. This would indicate that the test subject has an extremely high likelihood of both a pregnancy and a Zika infection, which would have resulted in a warning to seek medical attention at the conclusion of the tests. Other information may also be stored in the database in relation to the biologic, including other condition ratings, time and date each test was performed, user information such as ethnicity, gender, and age, and status indicators such as whether a test subject visited a physician as a result of the tests. The database **1204** thus provides the test subject with a growing collection of information that may be accessed by the test subject. This allows the test subject to present the test results to her physician for medical attention or additional testing, and allows for others who may access the database, such as disease researchers, to have access to data on various biologic samples and their markers.

**[0097]** Referring now to FIG. **14**, there is illustrated a flowchart of one embodiment of a biologic data collection and dissemination process **1400**. The process **1400** begins at step **1402** where a user of a testing device collects a biologic sample for use in a test or a series of tests. At step **1404**, the test or series of tests are performed on the biologic sample. At step **1406**, a mobile device application checks the biologic sample the testing device result to determine a quan-

titative result of the test to provide a correlative value for the condition being tested in the biologic sample. At step 1408, the test results and correlative values, or multiple values if multiple tests on the biologic sample were conducted, are transmitted to the remote server 1206. At step 1410, the biologic sample is given a unique identification number in the database 1204. At step 1412, the test results and correlative value or values are stored in the database 1204 in association with the unique identification number given to the biologic sample collected and in association with the particular tests performed. This way, the particular biologic sample may have various characteristics stored and retrieved in association with the biologic sample, and the test results may also be retrieved when data on a particular test is needed on a cross-section of users.

[0098] At step 1414, the results are provided to the user on the user's mobile device. At step 1416, the results are provided to the user's healthcare provider. The healthcare provider may receive the test results due to a visit from the user, the user bringing the results of the test with her on her mobile device, or the healthcare provider may receive the results from the database 1204 if the healthcare provider has permission to access the database 1204, or if access is granted in anticipation of the user's appointment with the healthcare provider. At step 1418, the test results are also provided to other healthcare industry individuals and organizations, including medical researchers, hospitals, and others.

[0099] Referring now to FIG. 15, there is illustrated a perspective view of a system for scanning test strips. The housing 602, as described hereinabove with respect to FIG. 6, is illustrated as being disposed within a slot 1502 in a test housing 1504. The test housing 1504 is connected through a line 1506 to a PC 1508. When the housing 602 containing the test strips 604 after being subjected to the biologics is inserted within the slot 1502, the test housing 1504 will scan the test strips 604 and analyze the results with the PC 1508. The PC 1508 will run some type of algorithm that can analyze the results of both of the test strips 604. There can be provided to indicators 1510 and 1512 on the surface of the test housing 1504, one being, for example, a ready LED and one being a green LED. The PC 1508, after analyzing results, can then provide a warning indicator such as lighting up the green LED for a positive indication of pregnancy and the red LED for indicating that there is some issue. As an example, suppose that the second test strip tested for the Zika virus. If so, a warning would be appropriate to output and activate the red LED. There could be any other type of indicator associated with the second test at 604 that, in a combination with the test results of the first test strip, i.e. for testing for the presence of a pregnancy state, testing for such things as diabetes, etc. Further, although only two test strips 604 are illustrated, there could be multiple test strips testing for many different biological issues that may be present in an individual. In this embodiment, by inserting the housing 602 into the test housing 1504 and allowing the PC 1508 to analyze the results, the indicators associated with the test strips can be analyzed with the assumption that all of the test return results were associated with an individual and in proximate time to each other. That means that the individual patient applied biological specimens, such as urine, blood, etc., to the appropriate test strips and, since these were all contained within the same test strip housing 602, this provides an indication that they are associated with a single

patient. Further, the test performed will typically be a test that will provide a very short-term response. Thus, the specimens can be applied to the test strips 604 in the test strip housing 602 and then inserted within the slot 1502 for testing by the PC 1508.

[0100] Referring now to FIG. 16, there is illustrated a cross-section of the test housing 1504. It can be seen that the test strip housing 602 is passed in slot 1502 past the camera 1602. The camera 1602 is operable to scan a small cross-section of the test strips 604 on the surface thereof as the test strip housing 602 passes thereby. Of course, there could also be a much larger camera provided for taking an entire image of the test strips 604 after being inserted within the test housing 1504. The camera 1602 is connected via a wire 1604 to an electronics package 1606 to process the information and send it to the PC 1508. The electronics package 1606 will also drive the indicators 1510 and 1512.

[0101] Referring now to FIG. 17, there is illustrated one embodiment of a vertical flow immunoassay device 1700. It will be understood that testing device 300 and other embodiments herein illustrate a lateral flow immunoassay device. However, other types of immunoassay devices may be used. For example, vertical flow immunoassay devices may be used, a two-sided flow through assay, or even a sandwich ELISA test may be run.

[0102] The testing device 1700 includes a housing 1702 that forms the body of the testing device. The housing 1702 may be made of plastic, metal, or any material durable enough for shipping and subsequent handling by a user. The housing 1702 may be hollow so that a plurality of immunoassay test pads 1704 may be housed within and so that a biologic may be deposited within the housing 1702. The testing device 1700 may further have a plurality of sample wells 1706, each sample well having one of the plurality of immunoassay test pads 1704 disposed within, and allowing for a user to view at least a section of a nitrocellulose membrane of each of the immunoassay test pads 1704, the membrane having a test line 1708 and control line 1710. The testing device 1700 may also have disposed on the surface of the housing a crosshair symbol 1712, used as an alignment target. This symbol may be a graphic printed or adhered to the testing device 1700. The crosshair symbol 1712 is used to align the testing device 1700 for the taking of an image of the testing device 1700 using a camera on a mobile device, for use in a mobile device application described herein. In other embodiments, the crosshair symbol 1712 may be other types of symbols, such as a simple shape (circle, square, etc.), other images (such as a medical cross symbol, an arrow, etc.), or any other type of image. In other embodiments, the device 1700 may be configured in such a way as to allow a biologic sample to be deposited into a sample well, and to present the results of the test on the opposite side of the housing. Such a configuration would allow the biologic to flow through the testing pad within the housing, with the reaction occurring on a reactive membrane on the side of the device opposite the sample well, with the device having a window for viewing the results.

[0103] Referring now to FIG. 18, there is illustrated a cross-sectional view of one embodiment of the vertical immunoassay device 1700. There is shown one of the plurality of immunoassay test pads 1704 residing within the housing 1702 below one of the plurality of sample wells 1706. The one of the plurality of immunoassay test pads 1704 includes an immunoreactive membrane 1802, such as

the nitrocellulose membranes disclosed herein. The immunoreactive membrane **1802** may have particle conjugates disposed thereon that binds when a biologic sample is received onto the immunoreactive membrane **1802** via the sample well **1706**, if the biologic sample contains the antigens or antibodies, or other indicators, for which the test is configured. The one of the plurality of immunoassay test pads **1704** also includes an absorbent pad **1804** for collection of excess biologic sample. It will be understood that the cross-sectional view illustrated in FIG. **18** shows one well of the plurality of sample wells **1706**. The other wells included in the device **1700** would be configured in a similar manner as that shown in FIG. **18**. There may also be included in the device **1700** an inner separating wall between each of the plurality of immunoassay test pads **1704**, to ensure that excess biologic material that is not adequately absorbed by the absorbent pad **1804** does not contaminate neighboring immunoassay test pads.

[0104] Referring now to FIG. **19**, there is illustrated a color gradient chart **1900**. When the mobile application described herein captures an image of the testing device, in some embodiments each pixel that makes up the test line captured in the image is processed to place it on a color gradient scale. In some embodiments, this placement may be done by examining the RGB values of the pixel. For any given test, there may be a visual color indicator (such as a test line) presented to the user of the test to indicate whether a reaction occurred. The color that is to be presented is known for the given test. Additionally, in some embodiments, the strength of the reaction will affect the strength of the color indicator. For example, if a test is supposed to produce a brown colored indicator, an image can be taken of the colored indicator to examine each pixel of the colored indicator to determine the strength of the color produced on the testing device, which indicates the strength of the reaction, and thus the risk level for the user.

[0105] The embodiment illustrated in FIG. **19** uses as an example a set of pixel RGB results for a test that produces a red colored indicator on the test strip when a reaction has occurred. There can be seen an origin point **1902** on the chart **1900**, wherein the RGB value is (255, 255, 255) or white. This may represent a no reaction state for the test strip, since the test line on the strip may only appear as a white blank space if no reaction has occurred. An x axis **1904** represents the color green, wherein the amount of green in the pixel decreases as it moves away from the origin in relation to the x axis **1904**. A y axis **1906** represents the color blue, wherein the amount of blue in the pixel decreases as it moves away from the origin in relation to the y axis **1906**. A diagonal line **1908** running in between the x axis **1904** and the y axis **1906** represents the color red, wherein the diagonal line **1908** running through the center of the chart **1900** is a maximum red color all along the diagonal line **1908**. If a pixel has less red than a 255 value, the pixel would be plotted away from the diagonal line **1908** in relation to whichever color is more predominant. For instance, if the pixel has RGB values of (127, 50, 205), a shade of purple, the pixel would be plotted somewhere in the lower right quadrant of the chart **1900**. FIG. **19** further illustrates an example plurality of pixel plot points **1910**, connected by a curved line, wherein the example plurality of pixel plot points **1910** shows test results that likely indicate a positive reaction, as the plot

points are all located near the diagonal line **1908**, demonstrating that the colored indicator was a heavy red color for the most part.

[0106] Referring now to FIG. **20**, there is illustrated a normalized past tests results chart **2000**. The captured pixels may be normalized into a single value for determining whether there is a likelihood of infection, pregnancy, or whatever else the test is designed to detect. This may be done in various ways. For example, the shade of red in all the pixels may be averaged to reach a single RGB value. Outliers may be left out so that the average is not heavily skewed, especially when there are few outliers present. This RGB value may then be given a value, such as a risk rating, ranging from 0 to 100. For example, an RGB value of (255, 255, 255) would be given a rating of 0. An RGB value of (255, 0, 0) would be given a rating of 100. An RGB value of (205, 150, 75) may be given a rating of 70, and so on. This normalized value may then be used to compare the user of the test to users of past tests to determine a risk level. In some embodiments, the control line and the test line may be captured and the results compared, as well. In addition, the real results of risk levels may also be used to adjust the stored normalized value. For instance, if a particular RGB value that seems to indicate a strong reaction repeatedly was found to not indicate an infection, this value may be adjusted to provide a lower risk rating. For instance, if a physician who saw a patient who had a (205, 150, 75) RGB value later reported to the operator of the server **1206** that further testing showed no infection was present, and if this trend continued substantially as reported by other physicians or medical organizations, subsequent test results by other test users that were near the RGB value of (205, 150, 75) may be given a lower rating.

[0107] Chart **2000** illustrates how past tests results may be collected and used to determine the risk of a current test user. A y axis **2002** represents a risk level rating, ranging from 0 at the origin to 100. An x axis **2004** represents time, wherein a plurality of normalized test results is plotted on the chart **2000**. The chart **2000** is further divided into sections across the y axis **2002**, indicating various risk level thresholds. For instance, and as illustrated in the chart **2000**, there may be at certain rating levels different thresholds of risk labeled as low, moderate, above average, and high risk levels. These thresholds may be moved over time as more data is accumulated via users conducting tests and the mobile application storing the data on the tests. When a user conducts a test, the user's normalized rating can be plotted similarly to past test results and weighed against them in order to provide a risk level for the user.

[0108] Referring now to FIG. **21**, there is illustrated the mobile device **802** displaying on the screen **804** a mobile application variable test functionality. There is displayed on the screen **804** a plurality of test functions **2102**. The plurality of test functions **2102** may be buttons that can be selected by a user to switch between tests within the mobile application. This allows for all test functions to be within the same mobile application. For each test run by the mobile application, data for the particular test chosen is utilized in performing the test, pulling the data from the remote server **1206**.

[0109] Referring now to FIG. **22**, there is illustrated the mobile device **802** of FIG. **8B**, wherein the housing **302** of the testing device **300** also includes thereon test function indicators **2202** and **2204**. The test function indicators **2202**



and **2204** are visual markers located on the housing **302** that identify to the mobile application the types of tests for which the testing device **300** is configured. These indicators may be any symbol, alphanumeric character, shape, etc. that can be added to the surface of the testing device **300**. The mobile application is programmed to recognize the indicator and perform the test function associated with the indicator. For example, the embodiment illustrated in FIG. **22** shows a “P” symbol for test function indicator **2202** and a “Z” symbol for test function indicator **2204**. In this embodiment, test function indicator **2202** indicates that one test strip in the testing device **300** is a pregnancy test, while test function indicator **2204** indicates that one test strip in the testing device **300** is a Zika test. This is used for merely illustrative purposes, and any recognizable symbol may be used for these two test functions, and any other type of test may have a symbol assigned in this way as well. Further, in some embodiments there may only be one indicator on the housing **302**, even if there are multiple tests. This single indicator would be for the combined test. For example, if the testing device **300** of FIG. **22** had a single symbol of “PZ,” this would indicate that the testing device **300** is a combined pregnancy and Zika testing device, allowing for the mobile application to recognize such and perform each test with knowledge of which strip is associated with which test based on the stored data on the testing device associated with the “PZ” symbol.

[0110] Referring now to FIG. **23**, there is illustrated the mobile device **802**, which in some embodiments is also used to users instructions on how to perform a self-diagnostic test. It is important for users to be able to use diagnostic test products correctly in order to obtain the most accurate results and to avoid possible injury to his or herself. Tests that require a blood sample for the biologic, for example, might require the user to prick his finger to obtain the blood. A user could cause injury to himself if this is not performed correctly. Or, providing the wrong type of biologic, saliva instead of urine, for example, to the sample well **308** or a test strip **100** would likely cause inaccurate results. For these types of reasons, it is important for the user to be able to perform the test properly. Various regulations also require that the users of self-diagnostic tests be sufficiently instructed on the proper use of the tests and testing procedures. In some embodiments, such as is illustrated in FIG. **23**, instructions for collecting performing the diagnostic test are provided by the mobile application in video and/or audio form. Before collecting the biologic and performing the diagnostic test, the user launches the mobile application on the mobile device **802**. The mobile application then provides the user with step-by-step instructions for the test. In the embodiment illustrated in FIG. **23**, a set of video instructions **2302** is presented on the screen **804**. The video instructions **2302** give detailed guidance on how to collect the biologic sample or samples and how to put the samples into the testing device **300**, as well as any other steps necessary for the test. In some embodiments, the mobile application includes controls **2304** which allow the user to play, pause, or replay the video instructions **2302** or parts of the video instructions. In some embodiments, the instructions for the diagnostic test are delivered by the mobile application on the mobile device **802** in an audio format. In these embodiments, the mobile application will still show various controls **2304** on the screen **804** which allow the user to play, pause, or replay the audio instructions.

[0111] In some embodiments, the file for the video or audio instructions are stored on the mobile device **802**, while in other embodiments, the files are stored on remote servers and then downloaded or streamed to the mobile device when the user wishes to view/listen to the instructions.

[0112] Turning now to FIG. **24**, there is illustrated an embodiment in which a mobile device **802** running the mobile application allows users to access test instructions by scanning a computer-readable code. In these embodiments, which allow users to receive instructions via video or audio formats as described hereinabove with respect to FIG. **23**, initiation of the instructions arises from scanning a code with the camera of the mobile device **802**. The mobile application allows for an image of a scan-able product code **2402**, which could be a bar code, a QR code, an alphanumeric code, or any other image than can be decoded by the application's software, to be captured by a camera on the mobile device **802**. The scan-able product code **2402** may be found on the exterior packaging of the product, on documentation included with the product, or even on some component of the self-diagnostic test product itself. The scan-able product code **2402** is linked to the particular type of self-diagnostic test with which the code was included. This allows the application software to determine which set of instructions need to be presented to the user. Similar to the testing device image capturing and image processing described hereinabove with respect to FIGS. **8A** and **8B**, the application displays a graphic **2404** which helps the user align the scan-able product code **2402** in the field of view of the mobile device **802** camera so that the camera can capture an acceptable image. When the scan-able product code **2402** aligns with the displayed graphic **2404**, the mobile application software recognizes this condition and captures an image of the product code. The mobile application then processes the image of the scan-able product code **2402** and accesses a database to find which set of instructions need to be presented to the user. In some embodiments, this database is stored in the software on the mobile device **802**, while in other embodiments, the database is stored on a remote server and is accessed by the mobile device through the internet. Once the mobile application has determined from the database which set of instructions need to be presented to the user, the application retrieves the instruction files from the mobile application or from the remote server and presents the instructions to the user, as described hereinabove with respect to FIG. **23**.

[0113] Turning now to FIG. **25**, there is illustrated another embodiment in which instructions for the diagnostic test are presented in an audio or video format by the mobile application. In these embodiments, rather than the user scanning a product code to inform the mobile application which set of instructions to present as described hereinabove with respect to FIG. **24**, the user inputs a code into the application. In these embodiments, a menu **2502** is presented on the screen **804** which allows the user to input an alphanumeric product code **2504** made of a combination of numbers and/or letters which indicate to the mobile application which instructions need to be presented. The alphanumeric product code **2504** may be printed on the packaging for the test, on documentation included with the test, or even on components of the test itself. Once the alphanumeric product code **2504** is input into the mobile application, the mobile application accesses

the database as described hereinabove with respect to FIG. 24 to retrieve or access the correct instructions to be presented to the user.

[0114] Turning now to FIG. 26, there is illustrated an embodiment in which the mobile application helps ensure that the instructions for the self-diagnostic test have been presented to the user. As discussed hereinabove with respect to FIG. 23, it is important, for various reasons, for the user of the test to fully understand the proper way to administer the test. To help ensure that the proper instructions for the test have been presented to the user, some embodiments include a feature which requires the instructions to be fully presented and for the user to acknowledge understanding the instructions. In these embodiments, the instructions for the diagnostic test are presented by the mobile application to the user in the manner described hereinabove with respect to FIGS. 23-25. The video or audio instructions must be presented in their entirety before the mobile application will allow the user to proceed to the part of the application in which the user captures an image of the testing device 300 to obtain a test result. Once the instructions have been fully presented to the user, the mobile application presents an acknowledgement menu 2602 to the user on the screen 804 of the mobile device 802. This acknowledgement menu 2602 requires the user to acknowledge that he has viewed (or listened) to the instructions and understands how to administer the self-test. The mobile application will not proceed to the step wherein the user captures an image of the testing device for image processing until the user acknowledges viewing (or listening to) and understanding the instructions. From the acknowledgment menu, the user can either select the option 2604 acknowledging he has viewed (or listened to) and understands the instructions, sending the application to the test device image capturing steps described hereinabove with respect to FIGS. 23-25, or the user can select the option 2606 which declines to acknowledge understanding the instructions. Selecting that option 2606 will cause the mobile application to re-present the instructions as described hereinabove with respect to FIG. 23, or cause the mobile application proceed to some stage of the application other than the test device image capturing stage.

[0115] Turning now to FIG. 27, there is illustrated a flowchart showing the process by which instructions are presented to the user via the mobile application. The process starts at block 2702, where the user starts the mobile application on the mobile device 802. The process then moves to decision block 2704. If the product code provided to the user is not a scan-able product code 2402, then the process moves to block 2706, where the user enters an alphanumeric product code 2504 into a menu 2502. The process then moves to block 2716, where the mobile application accesses a database and correlates the alphanumeric product code 2504 to the proper test instructions. If, at decision block 2704, the product code provided to the user is a scan-able product code 2402, the process instead moves to block 2708. Here, the camera on the mobile device 802 is activated, and an alignment graphic 2404 appears on the screen 804. Next, the process moves to block 2710, where the scan-able product code 2402 is aligned with the graphic on the mobile device screen 804 by the user. The process then moves to block 2712, where the mobile application causes the mobile device camera to capture an image of the scan-able product code 2402. Next, at block 2414, the mobile application processes the image of the scan-able

product code 2402 and processes it into a format which will be correlated with the database of instructions. The process then moves to block 2716, where the mobile application on the mobile device 802 accesses a database, locally or on a remote server, and correlates the formatted code to the proper instruction set in the database. Next, at block 2718, the mobile application retrieves the proper instruction files, either from the mobile device 802 or from a remote server via the internet. The process then moves to block 2720, where the instructions are presented to the user in either video or audio format. Next, the process moves to block 2722, where the application presents an acknowledgement menu 2602 to the user so that the user can acknowledge understanding the instructions. The process moves to decision block 2724, where, if the user does not acknowledge understanding the instructions, the process loops back to block 2720, where the instructions are again presented to the user. If the user acknowledges the instructions, the process moves to block 2726, where the mobile application allows the user to continue. The process moves to block 2728, where the user performs the self-diagnostic test, per the given instructions. The process then moves to block 2730, where the user scans the testing device 300 for results analysis. The process then ends at End block 2732.

[0116] It should be noted that, in some embodiments, the user will be taken to parts of the mobile application other than the playing of the instructions if the user declines to acknowledge understanding the instructions. For example, the mobile device 802 could present the user with a screen that reminds the user that the test cannot proceed until the user acknowledges understanding the instructions. The mobile application then gives the user another chance to acknowledge the instructions. Or, in other embodiments, the mobile application returns the user to the portion of the application where the user scans or inputs a code to allow the application to retrieve the correct instruction files.

[0117] In some embodiments, when the user acknowledges understanding the test instructions, a file or data log will be created to document that the user acknowledged understanding the test instructions. The log will include information such as the time at which the instructions were acknowledged, which diagnostic test the instructions were for, or which biologic ID the acknowledgement will be associated with. In some embodiments, the acknowledgement log is stored on the mobile device 802 in the mobile application software, while in other embodiments, the acknowledgement log is transmitted to a remote server for storage and record-keeping.

[0118] Turning now to FIG. 28, there is illustrated a flowchart for embodiments in which the image of the testing device 300 is processed by a database on a remote server, rather than by the mobile application itself running on the mobile device 802. These embodiments are useful for when a mobile application is capable of working with multiple different tests such that storing information and data needed to process several different types of tests might consume more data storage on a single mobile device than is practical or desirable. The process starts at Start block 2802, after the user has deposited the biologic sample into the testing device 300 and any chemical reactions have occurred. The process then moves to block 2804, where the mobile application activates the camera on the mobile device 802. The process moves to block 2806, where the user uses the mobile application to capture an image of the testing device 300

with the mobile device **802** camera. Next, at block **2808**, the mobile application communicates over the internet the image of the testing device **300**, along with information identifying the type of test being conducted, to a remote server and database for analysis. At block **2810**, the database analyzes the received test information and image and generates test results. This step is analogous to the steps described hereinabove with respect to FIGS. **9**, **11** and **14**, except that the image analysis takes place on a remote server and database, rather than on the mobile device itself. The process then moves to block **2812**, where the server communicates the test results back to the mobile application running on the mobile device **802**. The process then ends at block **2814**.

[0119] Turning now to FIG. **29**, there is illustrated a mobile device **802** from an embodiment which includes delivering audiovisual messages to a self-diagnostic test user in response to the user performing the test and submitting the test for results. After a biologic sample **202** is placed within the testing device **300**, a certain amount of time is required for the sample to migrate into the various parts of the strip or strips **204**, for any chemical reaction to occur, and for any visual indicators to appear in the testing device **300**. During this time, the user is somewhat of a “captive audience,” in that he will likely be focused on the test and the mobile application, rather than other aspects of daily life, while he is waiting for the test to be completed. This means that content providers of audiovisual messages know that their content is more likely to be paid attention to by the mobile application user. This, in turn, means that content presented to users can demand a premium price. Some embodiments of the system, such as that illustrated in FIG. **29**, take advantage of the user being a “captive audience” and allow the mobile application to present targeted audiovisual messages **2902** to the user. This occurs during the time between the user placing the biologic sample **202** in the testing device **300** and the time when the testing device is ready to have its image captured by the camera for analysis by the mobile application or remote server. In some embodiments, the targeted audiovisual messages **2902** are in the form a “TV channel” which provides health-related content and programming. This programming can include long-format video messages **2902** that are approximately thirty minutes in length such as might be found on a traditional TV channel and can resemble television shows or infomercials. The programming can also include audiovisual messages **2902** in the form of shorter video segments that are anywhere between one minute and five minutes in length. Some embodiments will present the same audiovisual messages **2902** to all users, regardless of which diagnostic test the user is performing. In other embodiments, the specific audiovisual messages **2902** presented to a particular user will depend on which diagnostic test the user is using. For example, if a user is performing a pregnancy test, the audiovisual messages **2902** will be related to babies or pregnancy. If a user is performing an HIV test, the audiovisual messages **2902** delivered to the user will be related to HIV treatment and management. Audiovisual messages **2902** can be created that relate to any of the types of tests found in various embodiments of the system.

[0120] Some embodiments will also include a countdown clock **2904**. The countdown clock **2904** is presented on the mobile device screen **804** while the biologic is moving through the test device **300** and any chemical reactions are

occurring, which is also when audiovisual messages **2902** are being presented to the user. The countdown clock **2904** displays the time until the test device **300** is ready to be photographed by the camera for processing by the mobile application or remote server. The inclusion of a countdown clock **2904** is another tool which helps keep the user focused on the mobile application while the audiovisual messages **2902** are being presented. In some embodiments, a countdown clock **2904** is presented to the user after any reactions have occurred and an image of the test device **300** has been captured by the camera. In these embodiments, the countdown clock **2904** displays the time left until the test device image is processed by the mobile application or the remote server and a result is delivered and presented to the user. The countdown clock **2904** is started by the user indicating through a menu that he has placed a biologic sample in the testing device **300**. It should be noted that the countdown clock **2904** is related to the time left for the reaction to complete (or the test device image to be processed), but in some embodiments, additional time is added to the countdown clock beyond just the completion time of the reaction or the image processing. In these embodiments, the countdown clock **2904** begins when the user photographs the testing device **300** for results analysis. Different types of self-diagnostic tests will have different test completion times. These times are stored in a database in the mobile application, or, in some embodiments, on a remote server which communicates the testing times to the mobile application.

[0121] In some embodiments, the audiovisual messages **2902** are presented to the user after the mobile device **802** camera has captured an image of the test device **300** for processing by the mobile application or the remote server and database. In these embodiments, the audiovisual messages **2902** that are presented after the user captures a test device **300** image are in addition to audiovisual messages presented while the user is waiting for any chemical reactions to take place in the test device before the image is captured. In still other embodiments, audiovisual messages **2902** are presented only after the image of the test device **300** is captured and is being processed by the mobile application or the remote server and database.

[0122] Turning now to FIG. **30**, there is illustrated a flowchart for the process of streaming audiovisual messages **2902** to a mobile application on a mobile device **802**. In some embodiments, the audiovisual messages **2902** are stored on the mobile device **802** itself. Preferably, however, the audiovisual messages **2902** are stored on a remote message database and then streamed by a server to the mobile device **802** which is running the mobile application. The process starts at block **3002** and proceeds to block **3004**, where the mobile application communicates information about the diagnostic test to the remote servers. This information notifies the server and database that the user is performing a diagnostic test and that the mobile application is ready to stream audiovisual messages **2902** to the user. For embodiments in which the audiovisual messages **2902** that are presented to the user are specific to the type of diagnostic test the user is performing, this information also includes information identifying the specific type of self-diagnostic test. Next, the process moves to block **3006**, where the testing time is determined from the diagnostic test identification information. In some embodiments, the testing time is communicated to the mobile application from a remote

server, while in other embodiments, this time is stored in a database within the mobile application. Next, at block **3006**, an appropriate audiovisual message **2902** or set of messages is selected from a message database. For embodiments which present specific messages **2902** to users of specific diagnostic tests, the test-identifying information is used by the database to select a message related to the type of test being used. The process then moves to block **3008**, where the remote server streams the audiovisual messages **2902** to the mobile device **802** running the mobile application. Next, at block **3010**, the mobile application presents the audiovisual messages **2902** to the user. The process ends at block **3012**.

[0123] Referring now to FIG. 31, there is illustrated a mobile device **802** from an embodiment in which video or visual advertisements are presented to the user in response to the user performing a self-diagnostic test. In these embodiments, the knowledge that the user has purchased and/or is performing a self-diagnostic medical test is used to deliver targeted advertisements **3102** to the user through the mobile application. Some embodiments store the files for the advertisements **3102** within the mobile application, while other embodiments allow the mobile application to stream or send the advertisements from a remote server. The targeted advertisements **3102** are presented to the user on the screen **804** of the mobile device **802** at different stages throughout the testing process. In some embodiments, the targeted advertisements **3102** will include generic advertisements **3102a** which are delivered to all users of the mobile application. These advertisements **3102a** are targeted at users of medical self-diagnostic tests generally, but are not specific to the type of test. Other embodiments will include targeted advertisements **3102b** which are directed at users of specific types of self-diagnostic tests. For example, a user who is performing a pregnancy test may see an advertisement **3102b** for a fertility clinic. As another example, a user who is performing a test for celiac disease may be presented with an advertisement for a brand of gluten-free food. Some embodiments will include advertisements in the form of electronic coupons **3104**. These electronic coupons **3104** allow users to "click" the coupon image on the mobile device screen **804** to receive coupons for health-related products and services. Different embodiments will allow users to receive coupons in different forms, such as redemption codes, physical coupons via mail, or computer readable images. Similar to the targeted advertisements **3102**, some embodiments will present the same electronic coupons **3104** to all users of the mobile application, while other embodiments will present different electronic coupons to users based on the type of diagnostic test being performed. Some embodiments also include advertisements in the form of informational links **3106** to various websites. These informational links **3106** present users with links to websites featuring informative literature or videos related to health issues and medical testing. Again, some embodiments will feature generic informational links **3106** common to all users of the mobile application, while other embodiments will present specific informational links to users of specific types of diagnostic tests.

[0124] As discussed hereinabove, the various types of advertisements **3102**, **3104**, **3106** can be presented to the user at different stages throughout the testing process. In some embodiments, the advertisements **3102**, **3104**, **3106** are presented when the user starts the mobile application. In

other embodiments, the advertisements **3102**, **3104**, **3106** are presented to the user when an image is scanned or a code is input by the user identifying the type of diagnostic test to the mobile application. In still other embodiments, the advertisements **3102**, **3104**, **3106** are presented to the user after the results of the test have been delivered to the user. Other embodiments will present the advertisements **3102**, **3104**, **3106** at other acceptable points in the testing process.

[0125] Turning now to FIG. 32, there is illustrated a flowchart which depicts the process for transmitting advertisements for embodiments in which the application downloads the advertisements **3102**, **3104**, **3106** from a remote server before presenting them to the user. The process starts at Start block **3202** and proceeds to block **3204**. At function block **3204**, the mobile application communicates to the server that a request for advertisements **3102**, **3104**, **3106** to present to the user. In embodiments in which the specific advertisement **3102**, **3104**, **3106** depends on what type of diagnostic test is being performed, the mobile application also communicates to the server information identifying the type of test. The process then moves to block **3206**. At block **3206**, the server accesses a storage database where the advertisements are stored and communicates the advertisements to the mobile device **802** running the mobile application. In embodiments which take into account the type of test being performed, the server selects appropriate advertisements **3102**, **3104**, **3106** from a database of advertisements based on the test identification information sent by the mobile application. The process then moves to block **3208**, where the files for the advertisements **3102**, **3104**, **3106** are communicated by the remote server to the mobile application on the mobile device. The process then moves to block **3210**, where the mobile application presents the advertisements **3102**, **3104**, **3106** to the user. The process then ends at End block **3212**.

[0126] Turning now to FIG. 33, there is illustrated an embodiment which displays advertisements along with audiovisual messages. These embodiments include the audiovisual messages **2902** as described hereinabove with respect to FIG. 29. However, these embodiments also include advertisements **3102**, **3104**, **3106** displayed on the screen **804** at the same time as the audiovisual messages **2902** are displayed, such as when the user is waiting for chemical reactions in the test to occur or for the processing of a test device image to complete. When advertisements **3102**, **3104**, **3106** are presented, they may be related to the audiovisual message **2902** also being displayed. For example, if the audiovisual message **2902** features actors discussing a particular medical or health product, the targeted advertisement **3102** could be an advertisement for that product. Or, if the audiovisual message **2902** features a short segment from a broadcast television show, the informative link **3106** could be a link to the website of the television show.

[0127] Turning now to FIG. 34, there is illustrated a mobile device **802** from an embodiment in which advertisements and other messages are delivered to the user based on the results of a self-diagnostic test. In these embodiments, targeted advertisements **3402**, electronic coupons **3404**, and informational links **3406** are presented to the user through the mobile application. These advertisements are similar to those described hereinabove with respect to FIGS. 31-32. However, the advertisements **3402**, **3404**, **3406** illustrated in FIG. 34 delivered to the user after the results of the self-

diagnostic test have been generated, and they are chosen based on the results of the test. These advertisements may include ordinary advertisements **3402** for products or services of interest for a person with the test result returned. The advertisements may also include electronic coupons **3404** for products or services of interest to individuals receiving the test result. Or, the advertisement may be an informational link **3406** directing the user to information relating to the test result he received. The common thread among the different types of advertisements **3402**, **3404**, **3406** is that the selection of the particular advertisements delivered to the user is influenced by the result of the diagnostic test. For example, if a user performed a diagnostic test for HIV, and the test showed a positive result for infection, the user would be presented with advertisements targeted toward an audience of HIV-infected individuals. These advertisements could include an advertisement **3402** for a HIV clinic, an electronic coupon **3404** for a discount on an anti-HIV drug, or an informational link **3406** for support groups for individuals infected with HIV. As another example, a user who receives a result from a pregnancy test showing that the individual is pregnant may be presented with maternity and baby-related advertisements **3402**, **3404**, **3406**, while an individual whose pregnancy test indicates the user is not pregnant may be presented with advertisements **3402**, **3404**, **3406** related to fertility clinics or adoption services.

[0128] Turning now to FIG. 35, there is illustrated a flowchart depicting the process for delivering advertisements in response to diagnostic test results. The process starts at Start block **3502**, where the user has already used the mobile application to capture an image of the test device **300** after the biologic sample has been placed in the test device. The process proceeds to function block **3504**, where the image of the testing device **300** is processed, either by the mobile application, or by a remote server. The process then moves to block **3506**, where a test result is generated based on the analysis of the processed testing device image. The process moves next to decision block **3508**. If the test results were generated the mobile application, the process moves to block **3510**, where the mobile application communicates the test results to a remote server, and the process proceeds to block **3512**. If the test results were generated by a remote server, the process moves from block **3508** to block **3512**. At block **3512**, the remote server accesses a database of advertisements and selects an advertisement or set of advertisements based on the results of the diagnostic test. The process moves to block **3514**, where the remote server communicates or streams files for the selected advertisements to the mobile device **802** running the mobile application. Next, at block **3516**, the mobile application presents the test result-specific advertisements to the test user. The process then ends at block **3518**.

[0129] Turning now to FIG. 36, there is illustrated an embodiment for a system which delivers content (advertisements, audiovisual messages, etc.) to users through a mobile application. The mobile application running on the mobile device **802** obtains identification information about the self-diagnostic test when the user scans an identification code on the product packaging or the testing device **300** itself (or, in some embodiments, when the user inputs a code). This identification information is communicated over a network **3602**, such as the internet, to a central office or remote server **3604** via Path (1). In some embodiments, the

information communicated by the mobile application also includes demographic information of the user, such as name, age, gender, geographic location, health history, diagnostic test history, or any other information which might be used in selecting advertisements. Using the test identification information sent by the mobile application on the mobile device **802**, the remote server **3604** accesses a database **3606**, which in some embodiments is on the remote server, and communicates back to the mobile application via Path (2) the time required for biologic sample to migrate through the testing device **300** and for any chemical reactions to occur. The time communicated by the remote server **3604** to the mobile application is used by the mobile application for the countdown timer **2904**. The central office or remote server **3604** uses the test identification (and in some embodiments, demographic) information communicated to it by the mobile application to select appropriate content from content contained in the database **3606**. In some embodiments, the content from database **3606** is of content accessed directly by the central office/remote server **3604**. In other embodiments, however, the content can be expanded by content providers **3608**. Each content provider **3608** is a third party database of content which can be used as advertisements, audiovisual messages, etc. by the mobile application. The content providers **3608** may be third parties who specialize in delivering content to users over the internet, such as YouTube, Hulu, Netflix, Amazon, Vimeo, or any other content delivery service. The content providers **3608** may also be producers of the content, such as television networks or product manufacturers or medical service providers. Once the central office **3604** has selected the appropriate content to be sent via an internal Path (3) to the mobile device **802**, the central office communicates this selection to the content database **3606** or the appropriate content provider **3608** via an internal Path (3). The content database **3606** or the content provider **3608** then sends or streams the files for the selected content to the mobile device **802** running the mobile application via a respective Path (4).

[0130] Turning now to FIG. 37, there are illustrated several example relational databases which are used in some embodiments to select appropriate content to be presented to the user of the self-diagnostic test by the mobile application. In some embodiments which send or stream content such as audiovisual messages or advertisements to the mobile application, the appropriate content is selected through the use of relational databases **3702** which correlate content to specific requirements or categories. For example, relational database **3702a** correlates the codes from different types of self-diagnostic tests to different content. Relational database **3702a** would be used for embodiments which present content based on the type of self-diagnostic test being used. Using the product number or code from a self-diagnostic test, a database such as database **3702a** allows the central office **3604** to determine which piece or pieces of content should be selected as appropriate for a user who is performing a particular self-diagnostic test. Other relational databases, such as database **3702b**, are used in embodiments which deliver content to users based on the results of self-diagnostic tests. In relational database **3702b**, content is correlated not only with the code from a specific type of self-diagnostic test, but also with a specific test result (such as "positive" or "negative") for that type of test. Relational database **3702c** correlates message run times with specific content. This allows content such as audiovisual messages to

be selected based on the time available for the content to be presented, as different types of tests will have different wait times between placing the biologic sample in the testing device 300 and when the testing device is ready to be photographed for analysis. Relational database 3702d correlates content with the content provider 3608 from which the content originates. This allows the central office 3604 to determine which content provider 3608 should be contacted when a specific piece of content is selected for delivery to a mobile application. A relational database 3702d is also useful for situations in which content from specific content providers 3608 is preferred for one reason or another, such as when one content provider has paid a premium to have its content prioritized for certain types of self-diagnostic tests, for example. Different embodiments will have different relational databases 3702. Some embodiments will have relational databases 3702 which correlate demographic data or users, such as age, gender, geographic location, health history, or diagnostic test history. Demographic relational databases are useful for embodiments in which the content which is selected is based at least partially on some aspect of the user's demographic data. For example, demographic data showing a user is a 27-year-old female may be more likely to be presented with an advertisement for a pregnancy test than a 63-year-old male.

[0131] Turning now to FIG. 38, there is illustrated a graph 3802 which depicts how a self-diagnostic test user's focus changes with time. A self-diagnostic test user only has a certain amount of attention and focus at any given time. This focus has to be divided among all of the things they are doing at that time. While the user is performing a self-diagnostic test, there will be certain times when their attention is focused almost exclusively on the testing device 300 as they wait for the results, and there will be other times when he is paying less attention to the testing device and can pay more attention to content such as advertisements and audiovisual messages being presented by the mobile application. Knowing when a user is mostly likely to be able to focus on the mobile device screen 804 as a function of the test environment in which they are in and any content that is being presented is valuable to content providers. On graph 3802 time  $t_0$  represents the time at which the user places a biologic sample in a testing device 300. Time  $t_1$  represents the time at which the testing device 300 is ready to be photographed for analysis. During the time between  $t_0$  and  $t_1$ , the ability of the user to focus on the screen will vary. In the example shown as graph 3802, the user has little attention to spend on the screen 804 at time  $t_0$ , as they are watching the testing device 300 where they just placed a biologic sample. As time progresses, they become less interested in the test device 300 and have more attention to focus on the screen 804. As time  $t_1$  approaches, however, the user quickly loses the ability to focus on the screen 804 as they anticipate the testing device 300 being ready to photograph. Knowing that at times approximately half way between times  $t_0$  and  $t_1$  give the user the most ability of focus on the screen 804, content providers might be willing to pay a premium to have their content presented to the user at these times, rather than near times  $t_0$  or  $t_1$ , when the user has less ability to focus on the screen. The content providers may also design their content to present the more valuable information to the viewer/user at the times determined to be associated with maximum focus.

[0132] Turning now to FIG. 39, there is illustrated an embodiment which includes a digital medical wallet and storehouse. Many retailers and manufacturers use "digital coupons" which consumers can redeem online or at physical retail establishments for products or service. Some retailers use customer loyalty programs which reward customers with "points" which can be redeemed for discounts or used as store credit. Typically, loyalty points, digital coupons, and digital store credit are associated with an account of some type, such as, for example, a customer's loyalty program for a chain of pharmacies. Therefore, these coupons and points can also be associated with an account linked to the user's mobile application information. A system which stores and keeps track of the various coupons and loyalty rewards for a consumer would enable the consumer to make better use of these coupons and points. In some embodiments, the mobile application on the mobile device includes a "wallet" which can store digital coupons and loyalty points and rewards for medicine and/or medical related products or services.

[0133] When a user wants to access any digital coupons or loyalty points associated with him or his account, he can open up the mobile application on the mobile device 802 and access the coupons/points. Similarly, when a user obtains a digital coupon or loyalty point, a record of such is stored in the mobile application (or on a remote server) as described hereinbelow. Referring again to FIG. 39, there is illustrated a mobile device 802 running a mobile application. The mobile application displays the digital coupons 3902 associated with the user. These digital coupons are redeemed in various ways, depending on the embodiment. Some embodiments allow the user to display the digital coupons on the screen 804 of the mobile device 802 and present the coupons to a cashier when the user is checking out at a retailer. Other embodiments present the user with a code which can be entered into a field in a web browser when the user is purchasing a product online. Loyalty points 3904 and store credit 3906 are also displayed by the mobile application. In some embodiments, the mobile application on the mobile device 802 keeps track of the loyalty points 3904 or the store credit 3906 associated with the user, while in other embodiments, the records for the points and/or store credit are stored on a remote server and transmitted to the mobile device 802 upon request by the mobile application. Upon checkout (either online or at a physical location), a user will be given the chance to use the redeem the loyalty points or store credit for eligible items or services.

[0134] Turning now to FIG. 40, there is illustrated an embodiment in which the mobile application stores a record of the medical supplies the user already owns. Often, when a patient goes to a healthcare provider, engages in a telemedicine session with a healthcare provider, or simply talks to a healthcare provider on the phone, the healthcare provider will recommend medication or some other type of treatment to the patient. Sometimes, these treatments will involve over-the-counter medications or treatments that the patient already owns. Therefore, it would be useful for a patient to have a way of knowing what medications and medical supplies he already owns. Some embodiments, such as that illustrated in FIG. 40, address this issue by keeping a database of medications and medical supplies (collectively referred to herein as "medications") that the user owns.

[0135] Referring still to FIG. 40, there is illustrated a mobile device 802 running a mobile application which is

displaying the various medications that the user owns. This “virtual medicine cabinet” displays icons **4002** for each different medication the user owns. When the user wants to check to see what medications he already owns, he simply opens the mobile application on the mobile device **802** and accesses the “virtual medicine cabinet” feature. The icons **4002** will display relevant information such as the name of the medication, the type of medication, its uses, or how much of the medication the user has. When a user purchases a new medication, he adds the medication to the “virtual medicine cabinet” (as described hereinbelow) so that it now has an up-to-date inventory of what medications the user has. Similarly, if a user runs out of a medication, he accesses the virtual medicine cabinet and removes the item from the inventory.

[0136] In some embodiments, the virtual medicine cabinet is shared with the user’s healthcare provider. In other words, the user can allow the healthcare provider to access the virtual medicine cabinet to see which medicines the user owns. This provides the benefit of the healthcare provider being able to, when appropriate, advise the user to use medications the user already has. Or, even if a prescription medication or an over-the-counter medication that the user does not have is the best option, the healthcare provider can recommend a temporary or supplemental medication to the user based on what the user already owns. For example, if a user has a sore throat, a healthcare provider may recommend, based on knowing that the user has a supply of pain relief tablets, that the user take one of the pain relief tablets for temporary relief until the healthcare provider can give a full diagnosis for the user’s sore throat. In some embodiments, the user can transmit the data in the virtual medicine cabinet to the healthcare provider, for example, by sharing the information with the healthcare provider during a telemedicine session. In other embodiments, the data for the virtual medicine cabinet is stored on a remote server which can be accessed by the healthcare provider.

[0137] Turning now to FIG. 41, there is illustrated an embodiment which allows a user to add medication to the “virtual medicine cabinet” by photographing the medication to be added. In these embodiments, the mobile application has the ability to capture an image of the medicine or the packaging the user uses the mobile application on a mobile device **802** to add the medication. The mobile application uses a camera on the mobile device **802** to capture an image of the medicine or medicine packaging. The software in the mobile application then analyzes the image and compares the image to information in a database to determine and recognize what the user captured an image of. In some embodiments, the mobile application recognizes text in an image, such as the name **4104** of the product from a label on the product, and compares the text to a database of known products. In other embodiments, mobile application has the ability to recognize and read barcodes on a product or product package. The mobile application then accesses a database to determine what medication the barcode is associated with. In some embodiments, the database to which the captured product images are compared is stored within the mobile application on the mobile device **802**. In other embodiments, however, the database is stored on a remote server. In these embodiments, the mobile application transmits the captured product image, or the information obtained from analyzing the image, to the remote server which compares the image or image information to the database to

identify the product. Once the mobile application or the remote server has identified the product, the mobile application displays to the user what it has identified the product as, allowing the user to confirm that it has correctly identified the product so that it can be added to the virtual medicine cabinet.

[0138] Turning now to FIG. 42, there is illustrated an embodiment of a system which includes a digital consumer wallet. First, the user uses the mobile application on the mobile device **802** to obtain digital coupons and/or loyalty points **4202**. The coupons can be obtained in various ways for different embodiments, such as downloading them from websites, scanning images of them from magazines or newspapers, or receiving them in emails. Loyalty or reward points are obtained in the manner chosen by the respective retailers, such as linking the mobile application to a customer loyalty account. For embodiments which store records of the digital coupons or loyalty points on a remote server, the records are transmitted through a network **4202** via Path ① to a remote central office **4206**. The remote central office **4206** then stores the coupon/loyalty points records in a connected database **4208**. In some embodiments, coupons are displayed on the mobile device **802** when the user is purchasing an item, allowing the user to show the coupon to the checkout employee or allowing the coupon to be scanned electronically. In other embodiments, such as when the coupons are used online, the coupon being redeemed is transmitted by the central office **4206** through the network **4204** via Path ② to the retailer **4210**. In embodiments in which retailers give coupons or loyalty points to the user based on the what the user has recently purchased, the retailer **4210** transmits the coupons/points through the network **4204** via Path ③ to the central office **4206**. The central office **4206** then notifies the user, through the network **4204** via Path ④, that he has received a new coupon or additional loyalty points. For embodiments in which the digital coupons **4202** are stored on a remote server **4206** and are redeemed via the mobile application on the mobile device **802**, the coupons are accessed by the mobile device by being transmitted via Path ④ through the network **4204** to the mobile device.

[0139] Turning now to FIG. 43, there is illustrated an embodiment of a system which provides a virtual medicine cabinet. In these embodiments, the user uses a mobile application on the mobile device **802** to scan the medical supplies **4102** that he currently owns. The mobile device **802** then transmits images or the information from the images of the medical supplies **4102** through a network **4302** via Path ① to a central office **4304**. The central office **4304** then stores the information about what medical supplies **4102** the user owns in a database **4306**. If the user wishes to access the virtual medicine cabinet to determine what medical supplies **4102** he already owns, the user sends a request to the central office **4304** via Path ①. The central office **4304** then accesses the database **4306** to determine the “contents” of the virtual medicine cabinet, and transmits the information through the network **4302** to the user’s mobile device **802** via Path ②. Should a healthcare provider **4308** wish or need to know what medical supplies **4102** the user currently owns, then the central office **4206** transmits the information detailing the contents of the virtual medicine cabinet to the healthcare provider through the network **4302** via Path ③. Naturally, the healthcare provider **4308** must be authorized

by or have been granted permission by the user to receive information about the user's virtual medicine cabinet.

[0140] Turning now to FIG. 44, there is illustrated a flowchart for an embodiment which includes a digital consumer wallet. The process begins at START block 4402 and flows to block 4404. At block 4404, the user obtains a digital coupon or loyalty points with a mobile application running on a mobile device, in any appropriate manner, such as those described hereinabove with respect to FIGS. 39 and 42. Next, the process moves to block 4406, where the mobile device transmits information regarding the digital coupons or loyalty points to a central office. The process then moves to block 4408, where the central office uses the information received from the mobile device to populate a database of coupons and/or loyalty for the user and associates the coupons/loyalty points in the database with the user. Next, at block 4410, the user or a retailer transmits a request to the central office for information regarding the coupons or loyalty points. One instance where this step would take place is when a user wants to redeem a digital coupon or a loyalty point. At block 4412, the requested coupon or point information is transmitted to the user or the retailer. In some embodiments, the information is transmitted to the mobile application on the user's mobile device, which can then be presented to a retailer. In other embodiments, the information is transmitted to the retailer itself at the request of the retailer or of the user. The process then ends at END block 4414.

[0141] Turning now to FIG. 45, there is illustrated a flowchart for an embodiment which includes a virtual medicine cabinet. The process begins with START block 4502 and proceeds to function block 4504. Here, the user uses a mobile application and a camera on his mobile device to scan the medical supplies the user currently owns. The process then moves to block 4506 where the mobile application processes the scanned images and uses an internal database to identify the objects in the images (or to correlate products to a scanned barcode for embodiments which include that feature). The process then moves to block 4508, where the mobile device transmits the inventory information, that is, the information about the medical supplies that were scanned, to a central office. The process then moves to block 4510, where the central office populates a database with the medical supply inventory information received from the user and associates the information with the user. Next, at block 4512, the user (through the mobile application) or a healthcare provider transmits a request for the inventory information to the central office. At block 4514, the central office transmits the contents of the virtual medicine cabinet to the user or the healthcare provider. The process then ends at END block 4516.

[0142] It should be noted that, in some embodiments, the images of products that are captured by the mobile device are not analyzed by the mobile application itself. Instead, in these embodiments, the images are transmitted by the mobile device to the central office. The central office then analyzes the images and correlates the information to information from a database to determine which product is in each image.

[0143] It should be understood that the drawings and detailed description herein are to be regarded in an illustrative rather than a restrictive manner, and are not intended to be limiting to the particular forms and examples disclosed. On the contrary, included are any further modifications,

changes, rearrangements, substitutions, alternatives, design choices, and embodiments apparent to those of ordinary skill in the art, without departing from the spirit and scope hereof, as defined by the following claims. Thus, it is intended that the following claims be interpreted to embrace all such further modifications, changes, rearrangements, substitutions, alternatives, design choices, and embodiments.

1. (canceled)
2. A system, comprising:
  - a mobile device; and
  - a server configured to:
    - receive, from a mobile device, diagnostic test results and user information associated with a testing device;
    - store the diagnostic test results and the user information on a server disposed on a network;
    - receive, from the mobile device, an image of at least one medical product;
    - identify the at least one medical product in the image;
    - populate a database with user medical supply inventory information including information associated with the identified at least one medical product; and
    - transmit at least a portion of the user medical supply inventory information to a healthcare provider.
3. The system of claim 2, wherein the server is further configured to:
  - receive, from the mobile device, loyalty point information;
  - populate the database with the loyalty point information in association with a user;
  - receive a request from a retailer for the loyalty point information; and
  - transmit the loyalty point information to the retailer.
4. The system of claim 2, wherein the testing device includes a plurality of immunoassay test strips.
5. The system of claim 4, wherein a test line of one of the plurality of immunoassay test strips includes Zika virus antigen and a test line of another one of the plurality of immunoassay test strips includes an antibody suitable for binding with hCG.
6. The system of claim 4, wherein the mobile device includes a camera, a viewing screen, and a software application stored thereon, wherein the software application provides executable instructions that, when executed, cause the mobile device to:
  - initiate operation of the camera of the mobile device;
  - present on the viewing screen of the mobile device an alignment graphic to be aligned with an alignment target of the testing device;
  - detect when an alignment of the alignment graphic and the alignment target has taken place;
  - capture an image of the testing device;
  - process the image to determine pixel count and line intensity of a test line of each of the plurality of immunoassay test strips;
  - compare one or more results of processing the image to a control for each test line of each of the plurality of immunoassay test strips; and
  - present test results on the viewing screen.
7. The system of claim 6, wherein the control is a dataset from previously conducted tests stored on a database and accessed by the software application.
8. The system of claim 6, wherein the test results include a quantitative result.



9. The system of claim 8, wherein the quantitative result includes a reaction rating.

10. The system of claim 2, wherein the server is further configured to:

determine if the diagnostic test results include a positive result;

present, if the diagnostic test results are positive, a telemedicine initiation option on a screen of the mobile device;

determine whether the telemedicine initiation option is selected;

send the diagnostic test results from the server to a telemedicine provider;

send additional medical history information to the telemedicine provider; and

initiate a telemedicine conference with the telemedicine provider.

11. The system of claim 10, wherein the server is further configured to:

receive, over a network, a notification relating to an issued prescription; and

communicate information relating to the issued prescription over a network to a pharmacy.

12. A method, comprising:

receiving by a server, from a mobile device, diagnostic test results and user information associated with a testing device;

storing, by the server, the diagnostic test results and the user information on a server disposed on a network;

receiving, by the server from the mobile device, an image of at least one medical product;

identifying, by the server, the at least one medical product in the image;

populating, by the server, a database with user medical supply inventory information including information associated with the identified at least one medical product; and

transmitting, by the server, at least a portion of the user medical supply inventory information to a healthcare provider.

13. The method of claim 12, further comprising:

receiving, by the server from the mobile device, loyalty point information;

populating the database with the loyalty point information in association with a user;

receiving a request from a retailer for the loyalty point information; and

transmitting the loyalty point information to the retailer.

14. The method of claim 12, wherein the testing device includes a plurality of immunoassay test strips.

15. The method of claim 14, wherein a test line of one of the plurality of immunoassay test strips includes Zika virus

antigen and a test line of another one of the plurality of immunoassay test strips includes an antibody suitable for binding with hCG.

16. The method of claim 14, wherein the mobile device includes a camera, a viewing screen, and a software application stored thereon, and the method further comprising:

initiating operation of the camera of the mobile device;

presenting on the viewing screen of the mobile device an alignment graphic to be aligned with an alignment target of the testing device;

detecting, by the mobile device, when an alignment of the alignment graphic and the alignment target has taken place;

capturing, by the mobile device, an image of the testing device;

processing, by the mobile device, the image to determine pixel count and line intensity of a test line of each of the plurality of immunoassay test strips;

comparing, by the mobile device, one or more results of processing the image to a control for each test line of each of the plurality of immunoassay test strips; and

presenting test results on the viewing screen of the mobile device.

17. The method of claim 16, wherein the control is a dataset from previously conducted tests stored on a database and accessed by the software application.

18. The method of claim 16, wherein the test results include a quantitative result.

19. The method of claim 18, wherein the quantitative result includes a reaction rating.

20. The method of claim 12, further comprising:

determining, by the server, if the diagnostic test results include a positive result;

presenting if the diagnostic test results are positive, a telemedicine initiation option on a screen of the mobile device;

determining whether the telemedicine initiation option is selected;

sending, by the server, the diagnostic test results from the server to a telemedicine provider;

sending, by the server, additional medical history information to the telemedicine provider; and

initiating, by the server, a telemedicine conference with the telemedicine provider.

21. The method of claim 20, further comprising:

receiving, by the server over a network, a notification relating to an issued prescription; and

communicating information relating to the issued prescription over a network to a pharmacy.

\* \* \* \* \*